





Current Data Parameters  
NAME 0816-4923  
EXNO 1  
PROCNO 1

F2 - Acquisition Parameters

Date 20240819  
Time 14:47 h  
INSTRUM spect  
PROBHD z16098\_0490 (z16098\_0490)  
PULPROG zgpg30  
TD 65536  
SOLVENT DMSO  
NS 16  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.244532 Hz  
AQ 4.0894465 sec  
RG 137.37  
DW 62.490 usec  
DE 6.50 usec  
TE 298.2 K  
D1 1.0000000 sec  
T1 400.1524709 MHz  
SFO1 400.1524709 MHz  
NUC1 1H  
P1 10.00 usec  
PKWA 14.69799995 W

F2 - Processing parameters

SI 65536  
SK 400.1500023 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GE 0  
PC 1.00

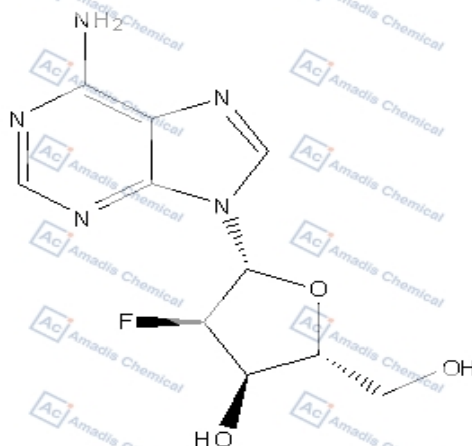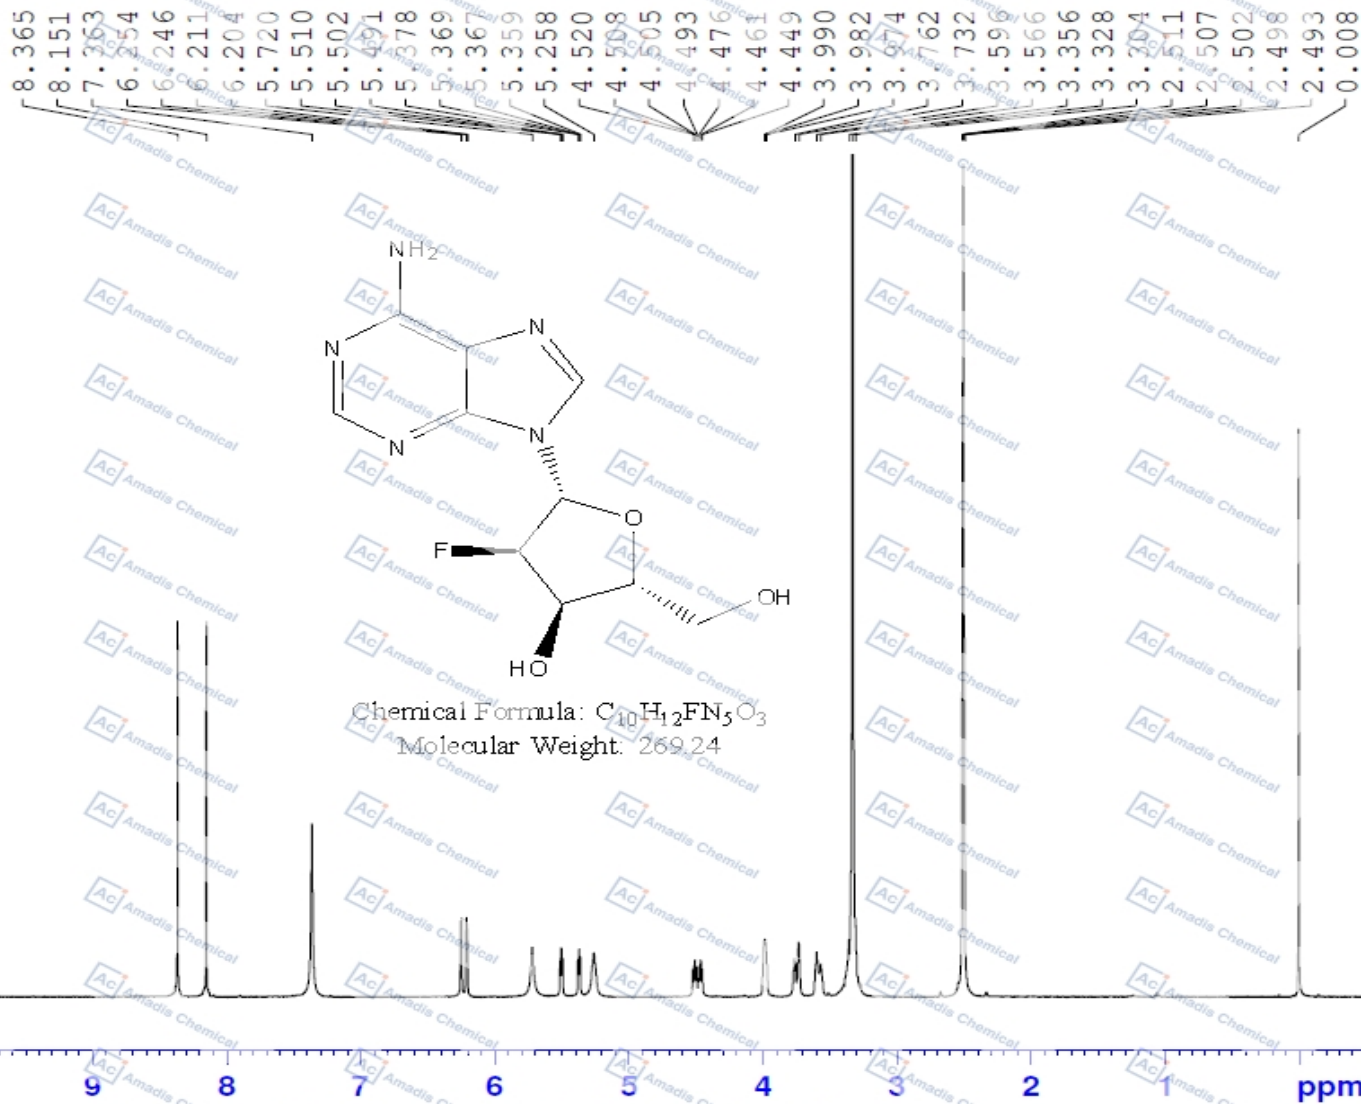

\*For laboratory or manufacturing use only, not for drug, food and household use.