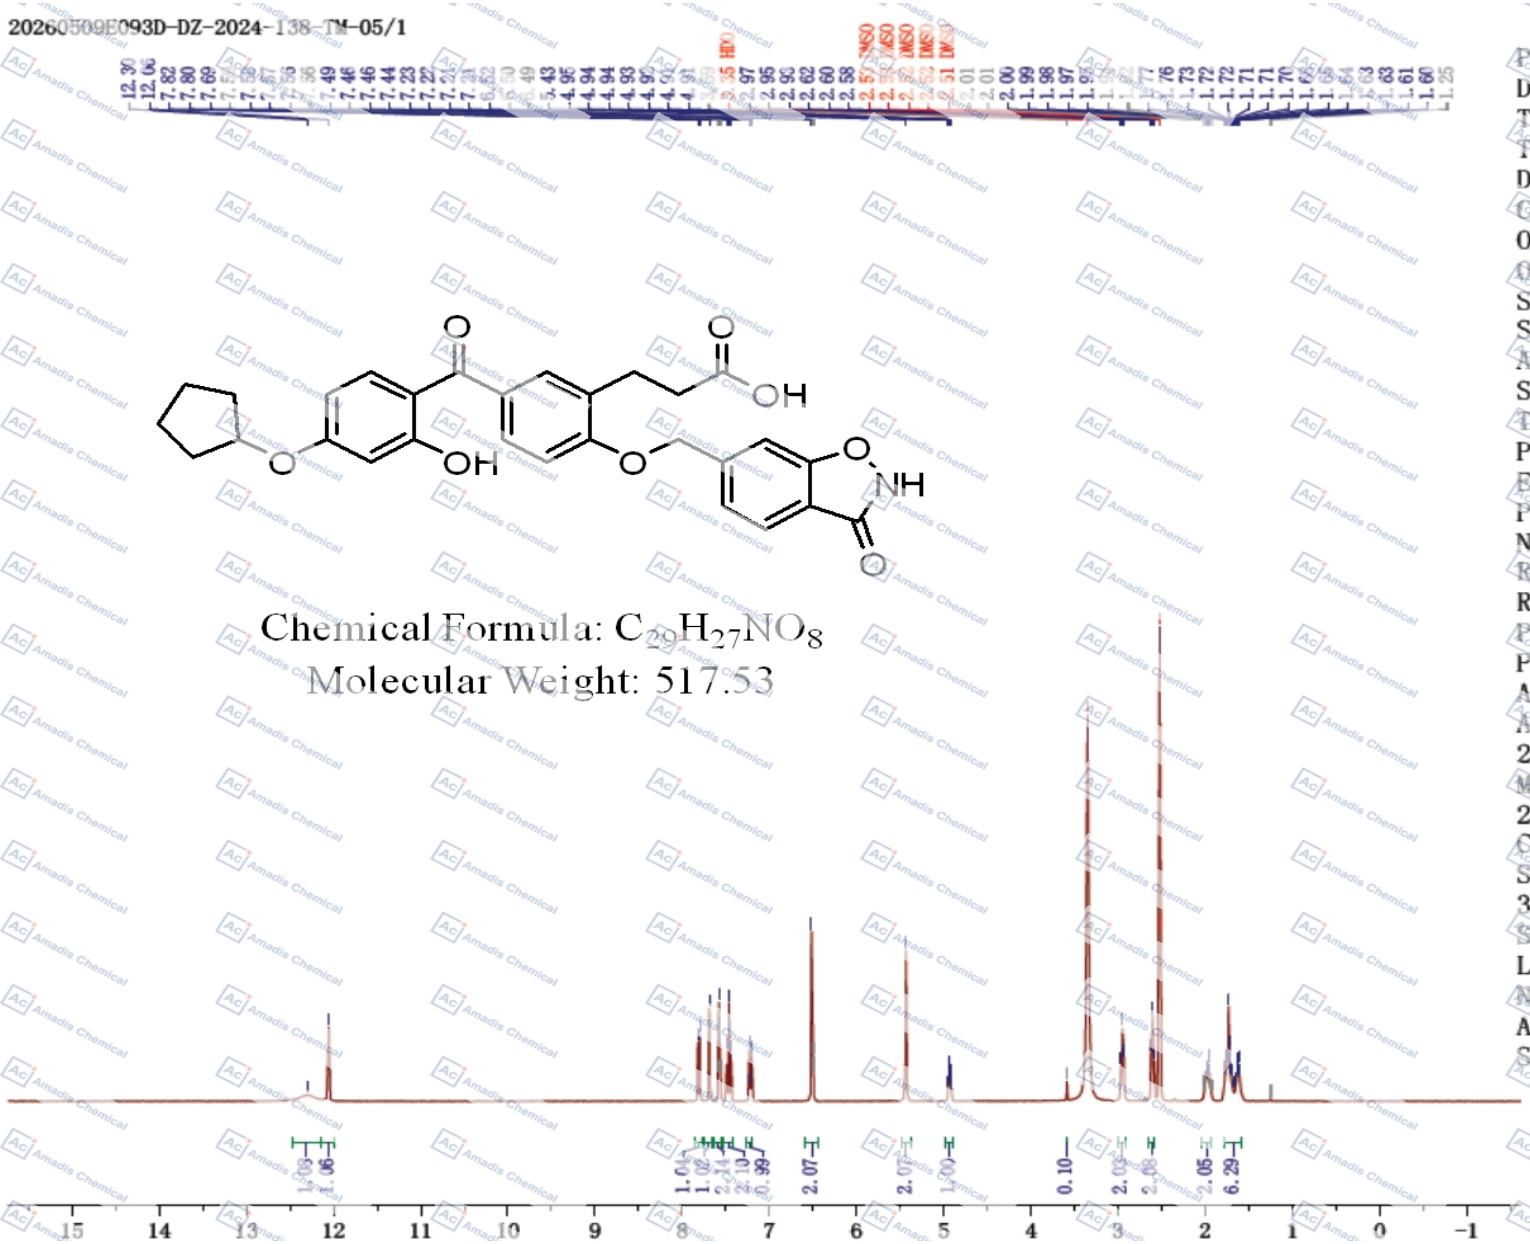

Parameter	Value
Data File Name	DZ-2024-138-TM-05/1/fid
Title	20260509E093D-DZ-2024-138-TM-05/1
Comment	
Origin	
Owner	guest
Site	
Spectrometer	QUANTUM-I
Author	
Solvent	DMSO
Temperature	298.1
Pulse Sequence	s1pul30
Experiment	1D
Probe	probeinfo
Number of Scans	8
Receiver Gain	55
Relaxation Delay	1.0000
Pulse Width	10.6000
Presaturation Frequency	
Acquisition Time	4.0002
Acquisition Date	2026-05-09T13:57:59
Modification Date	2026-05-13T10:23:22
Class	
Spectrometer Frequency	399.87
Spectral Width	8012.0
Lowest Frequency	-1606.7
Nucleus	1H
Acquired Size	32050
Spectral Size	65536

*For laboratory or manufacturing use only,not for drug,food and household use.