



Current Data Parameters

EXPNO 1
PROCNO 1


F2 - Acquisition Parameters

Time 12.52
INSTRUM spect
PROBHD 5 mm F4BBO BB/
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.22266 Hz
AQ 4.089465 sec
RG 81.42
DW 62.400 usec
DE 6.50 usec
TE 291.6 K
D1 1.0000000 sec
TDO 1

==== CHANNEL f1 =====
SFO1 400.1324710 MHz
NUC1 1H
P1 10.00 usec
PLW1 16.00000000 W

F2 - Processing parameters

SI 65536
SF 400.1300100 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

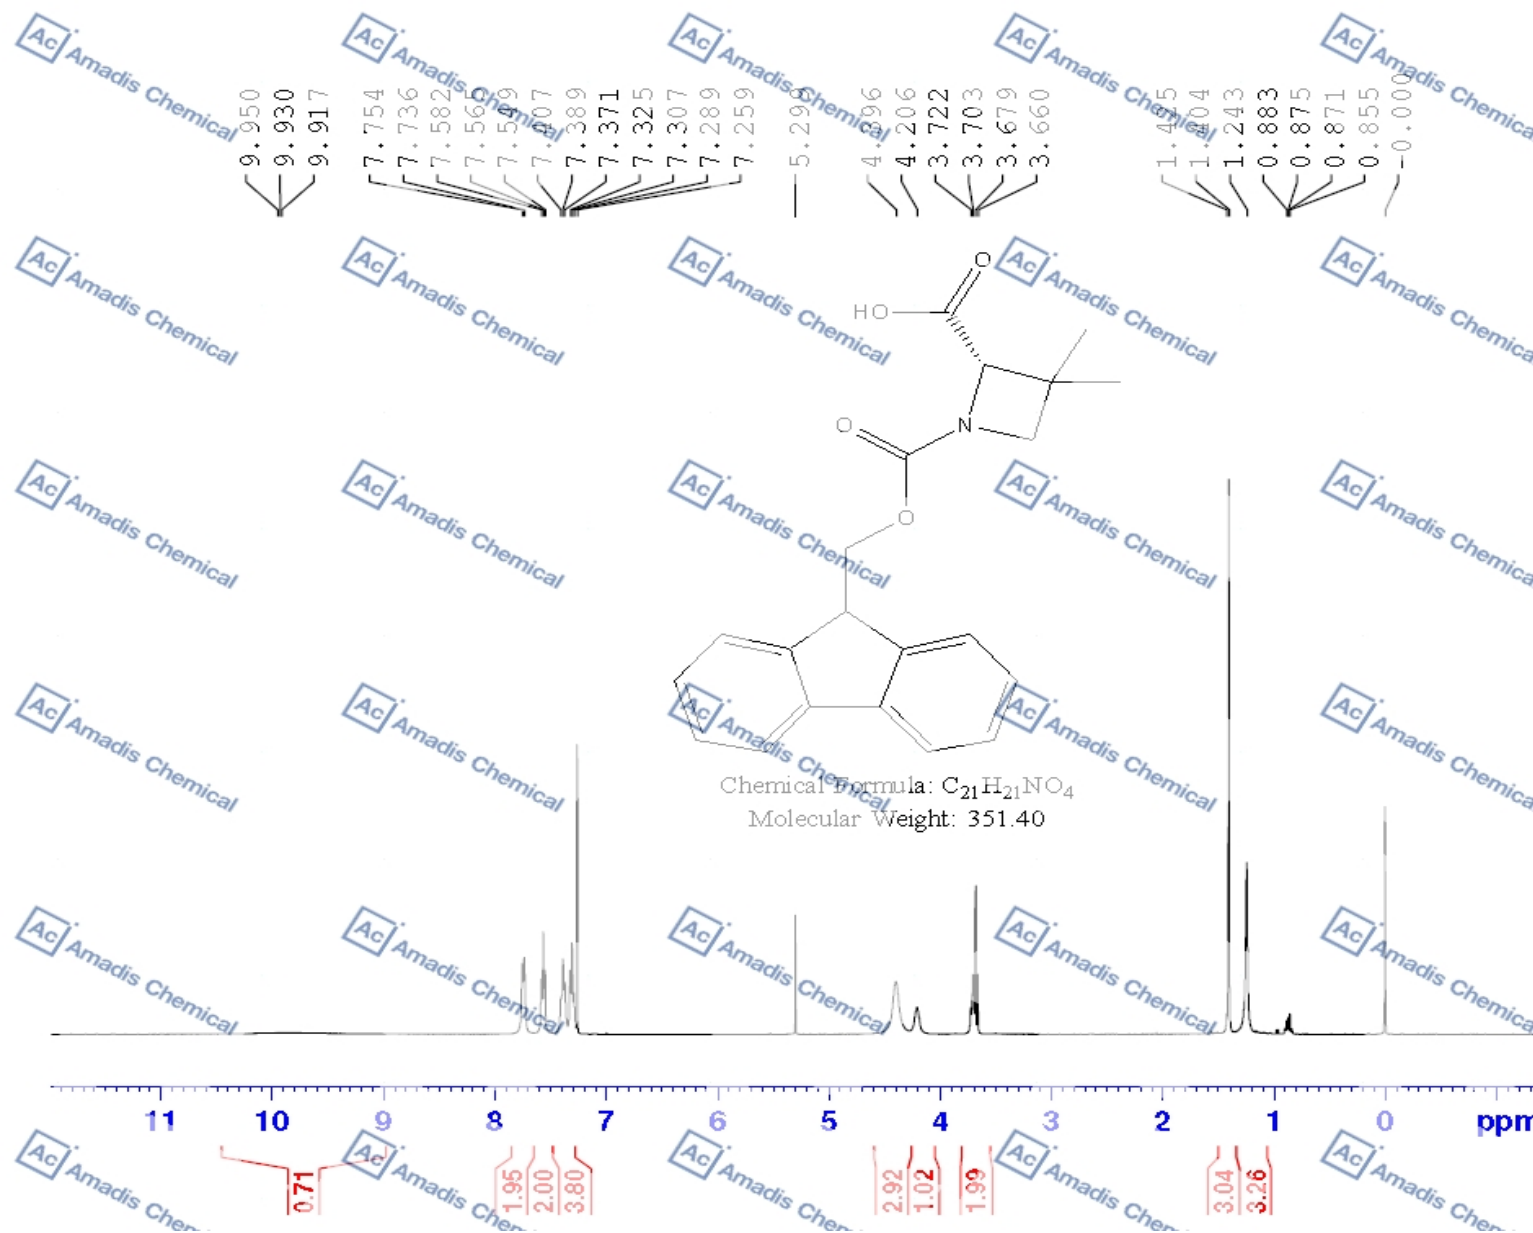

*For laboratory or manufacturing use only, not for drug, food and household use.