


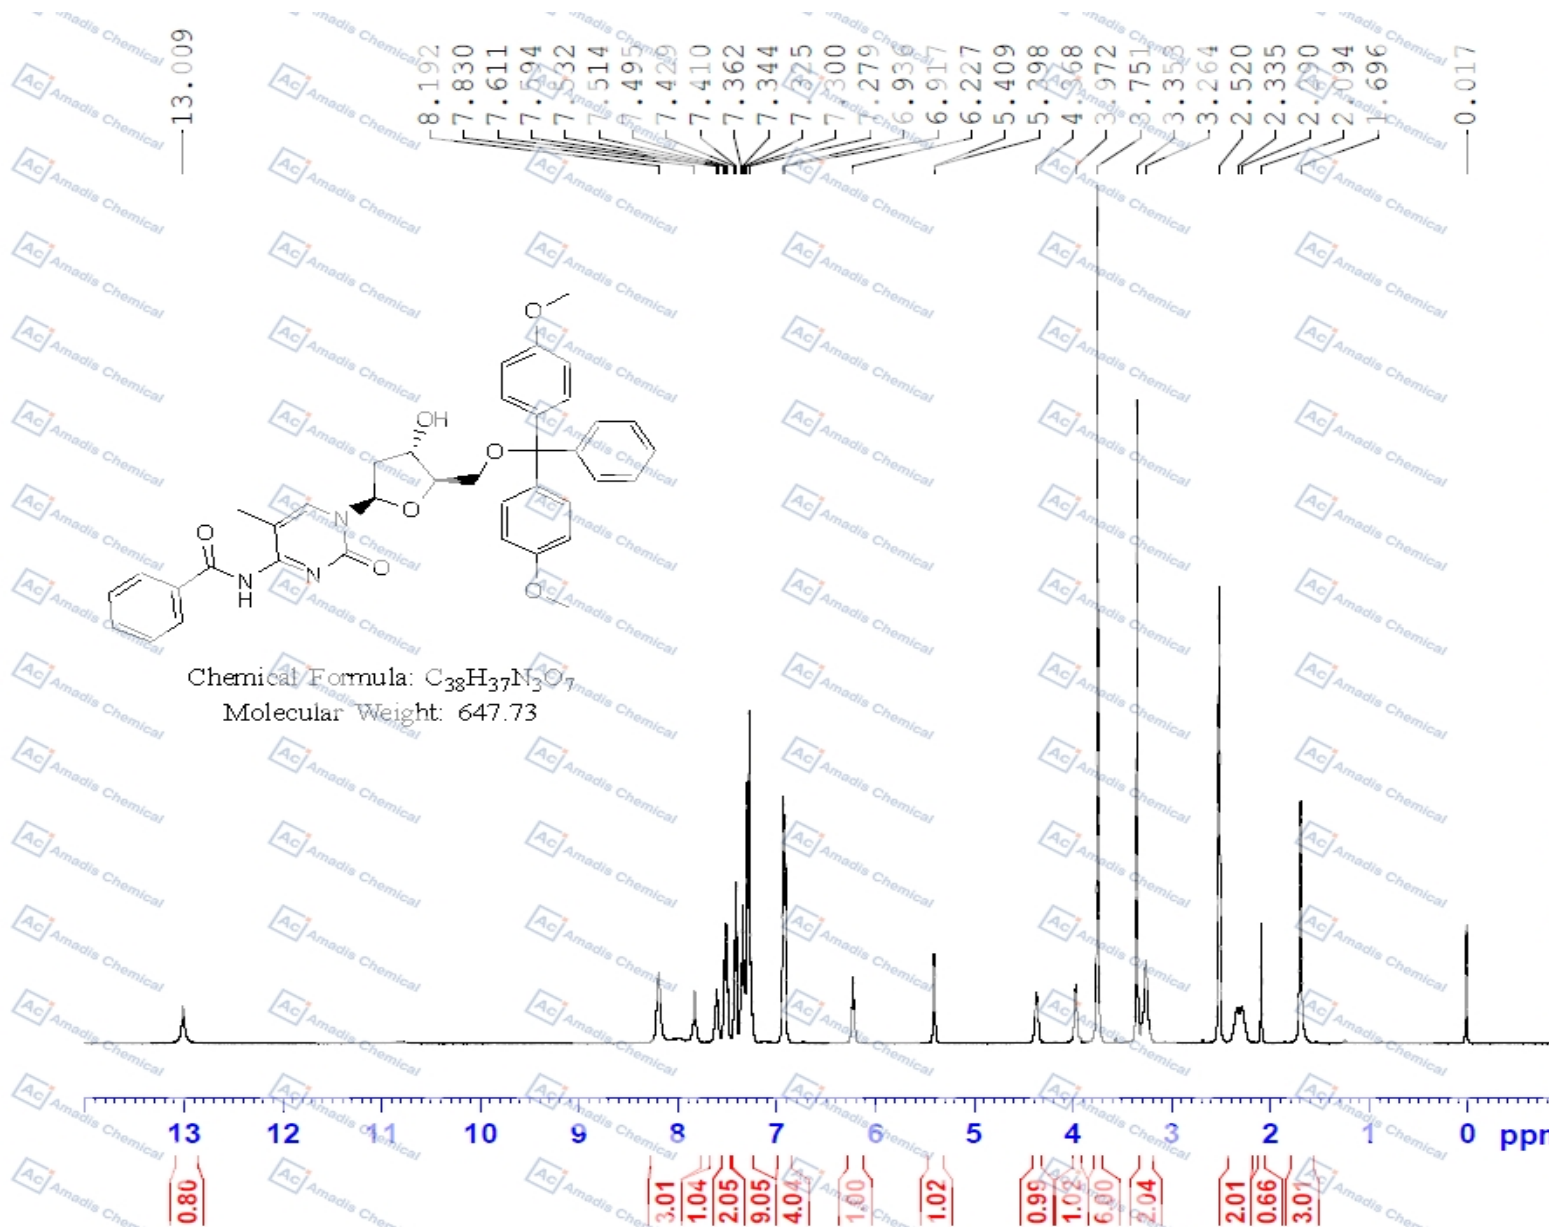

Current Data Parameters	
NAME	G1011-038-10
EXPNO	1
PROCNO	1
F2 - Acquisition Parameters	
Date_	20241207
Time	18.16
INSTRUM	QUANTUM-1
PROBHD	probeinf
PULPROG	sigul30
TD	65536
SOLVENT	DMSO
NS	16
DS	2
SWH	8012.000 Hz
FIDRES	0.124962 Hz
AQ	4.0002499 sec
RG	57.54
DM	62.406 usec
DE	30.00 usec
TE	273.1 K
NUC1	1H
SE01	399.8218529 MHz
SI	1.00000000 sec
P1	15.00 usec
PL1	45.00 dB
P1W	0.00021773 W
F2 - Processing parameters	
SI	65536
SE	399.8218539 MHz
WDW	EM
SSB	0
LB	0.30 Hz
GB	0
PC	4.00

*For laboratory or manufacturing use only, not for drug, food and household use.