


MS of 1951424-92-2

MASS SPECTROMETRY REPORT

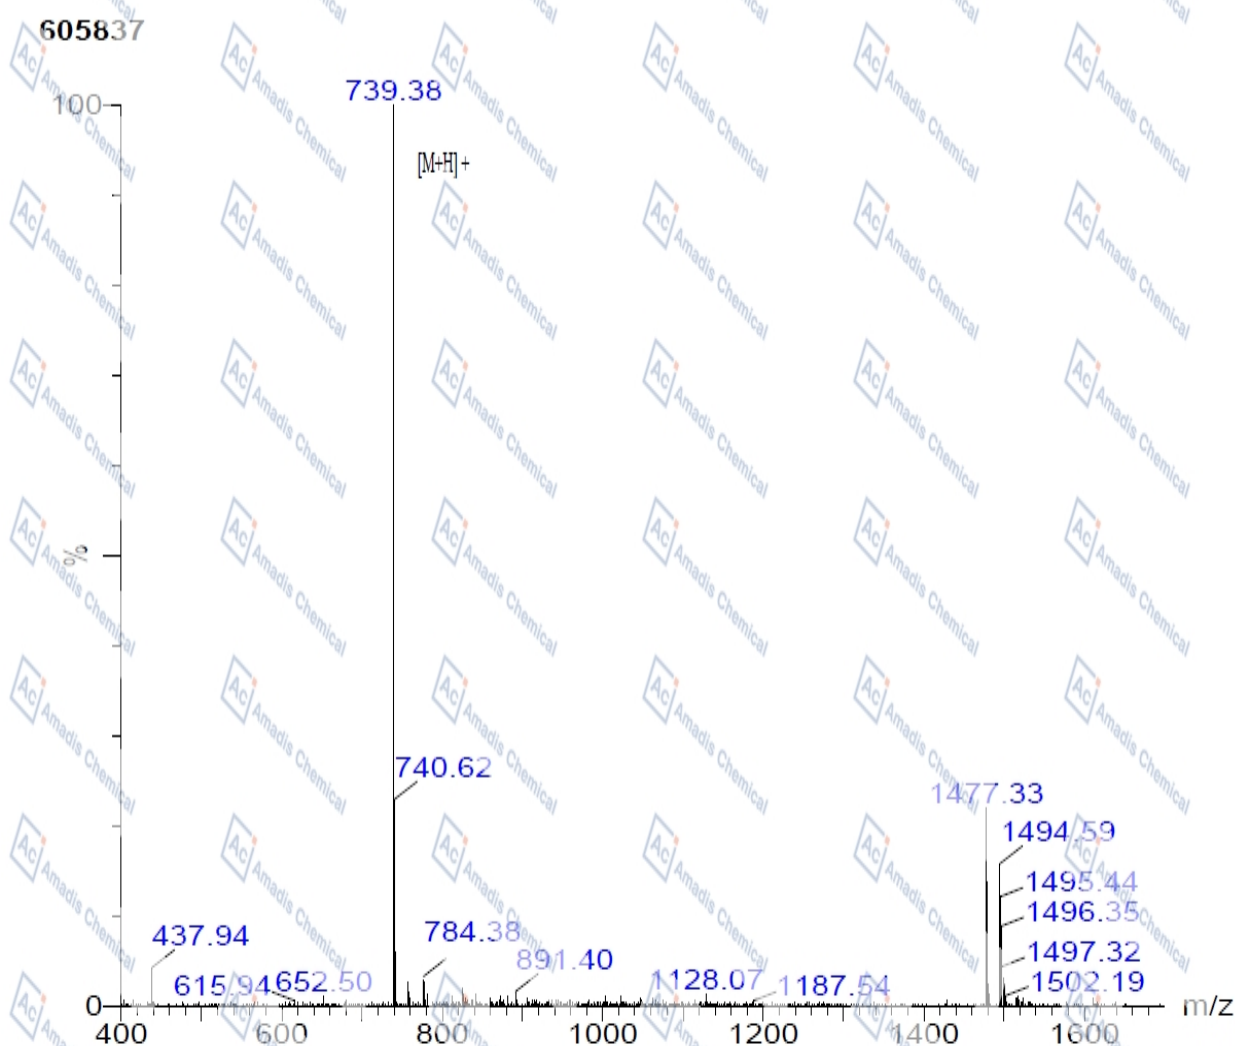

Sample Description

Analyst: SHAO
Sample: 605837
M.W.: 738.8
Lot. No.:

Instrument

Probe: ESI
Nebulizer Gas Flow: 10L/min
CDL: 52.0v
CDL Temp.: 350 °C
Block Temp.: 120 °C

Waters ZQ 2000

Probe Bias: +3.5kv
Detector: 0.05kv
T. Flow: 0.5ml/min
B. Conc.: 50%H₂O/50%ACN

*For laboratory or manufacturing use only, not for drug, food and household use.

* If you have any comments and suggestions, please contact us by sales@amadischem.com