



Current Data Parameters


NAME 0805-4909
EXPNO 1
PROCNO 1

F2 Acquisition Parameters

Date_ 20240806
Time 11.41
INSTRUM spect
PROBHD Z116098_0490
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 4
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 111.000
DW 62.400 usec
DE 6.50 usec
TE 298.6 K
D1 1.00000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PLW1 14.69799995 W

F2 Processing parameters

SI 65536
SF 400.1500014 MHz
WDW EM
SSB 0
LB 0.40 Hz
GB 0
PC 1.00

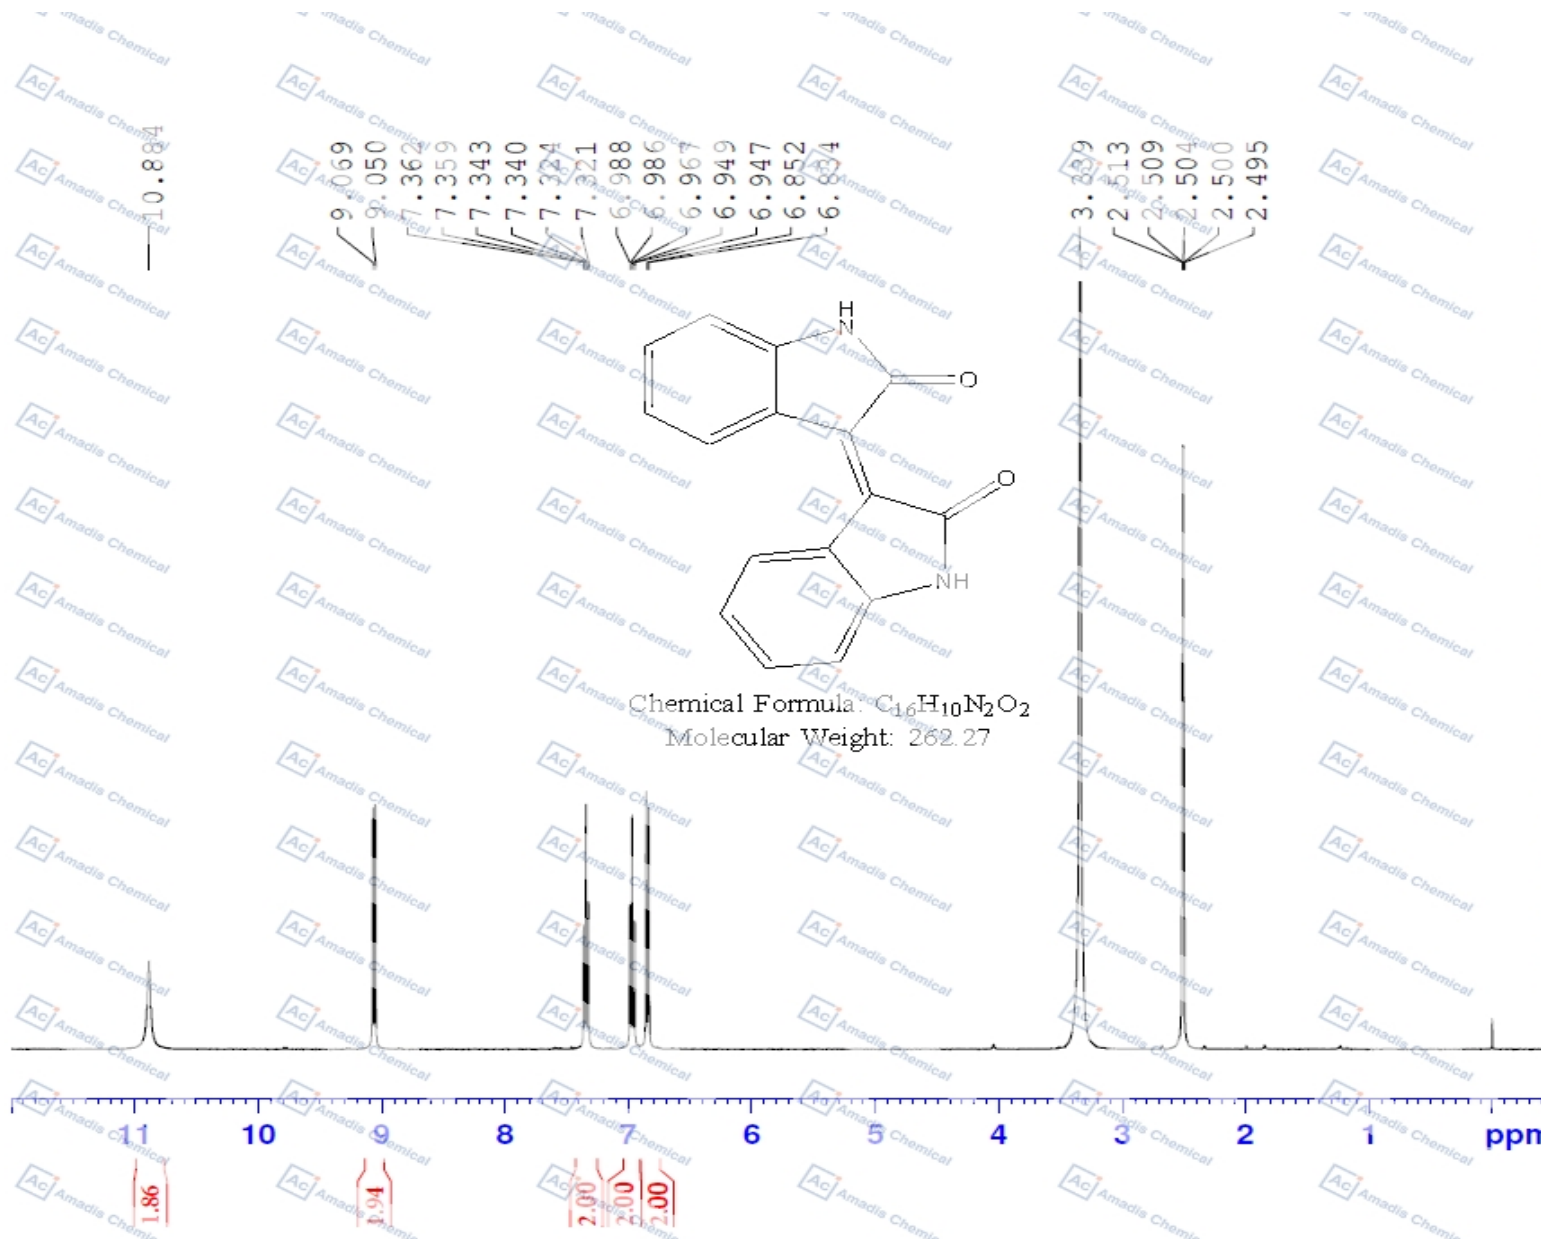

*For laboratory or manufacturing use only, not for drug, food and household use.