


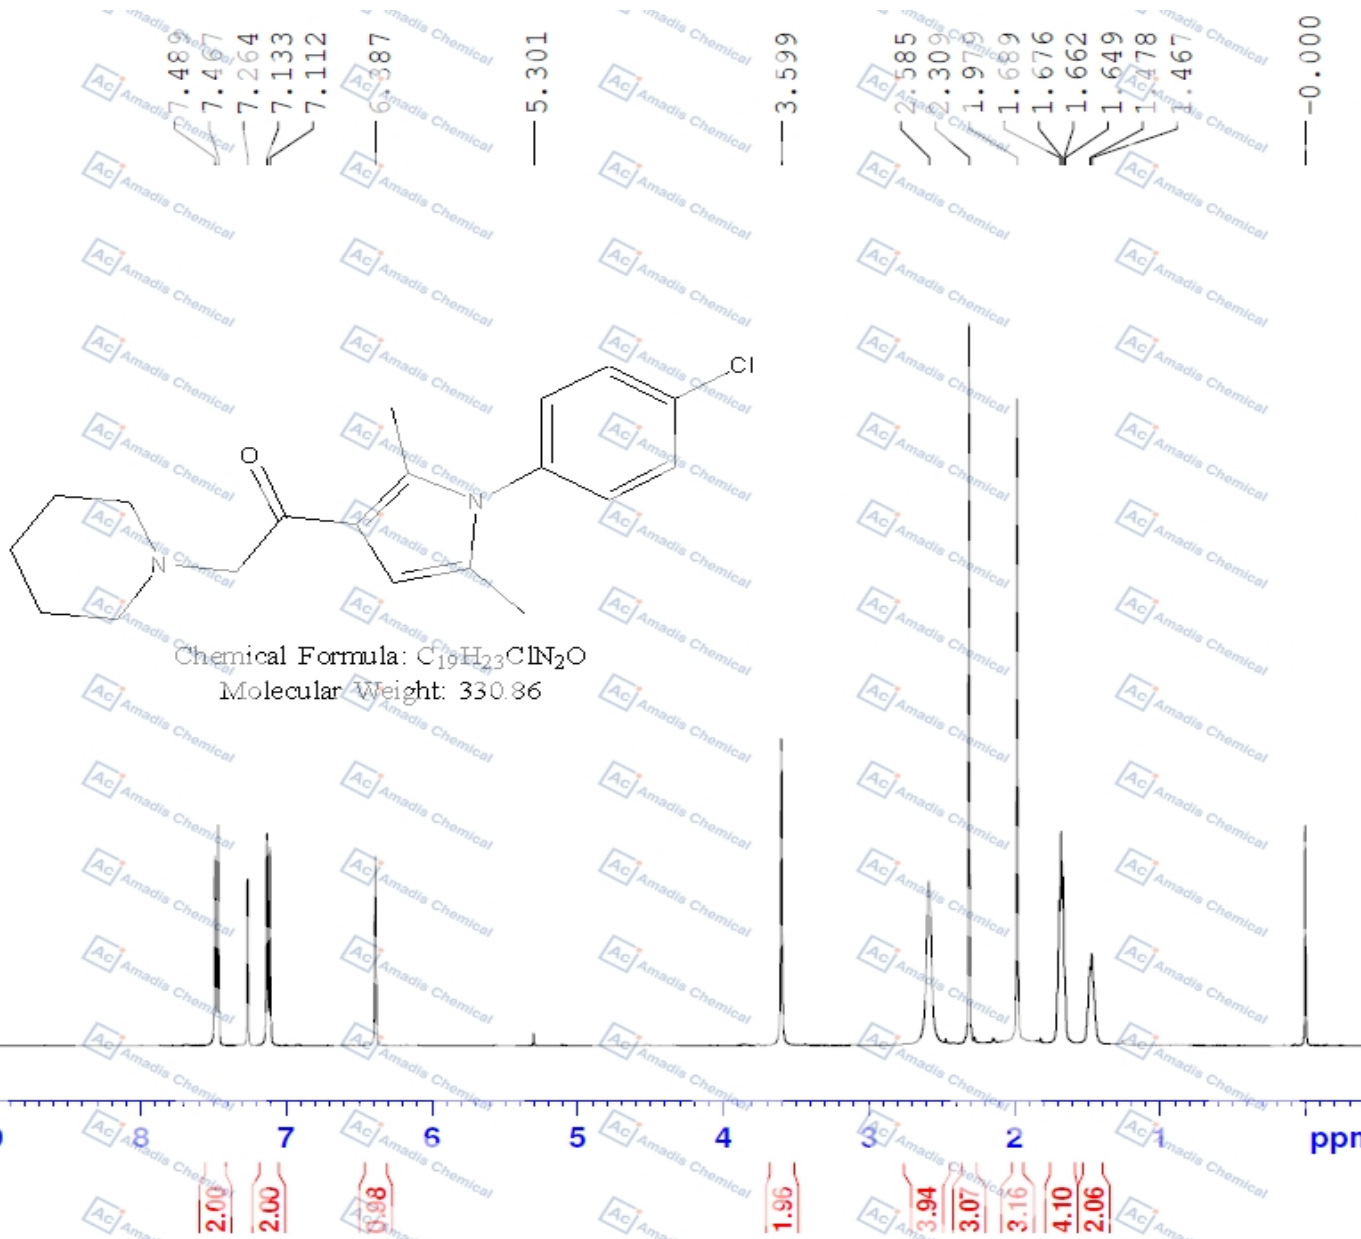

BRUKER

Current Data Parameters

NAME	1204-5086
EXPNO	10
PROCNO	1

F2 - Acquisition Parameters

Date_	20241205
Time	18:50 h
INSTRUM	spec
PROBHD	Z116098_0490
PULPROG	zg30
TD	65536
SOLVENT	CDCl ₃
NS	16
DS	2
SWH	80124.920 Hz
FIDRES	0.244532 Hz
AQ	4.0894465 sec
RG	111.92
DM	624.000 usec
DE	8.50 usec
TE	297.2 K
D1	1.00000000 sec
AD9	1
SFO1	400.1524709 MHz
NUC1	1H
P1	10.00 usec
PLW1	14.6978995 W

F2 - Processing parameters

SI	65536
CF	400.150084 MHz
WDW	EM
SSB	0
LB	0.30 Hz
GB	0
PC	1.00

*For laboratory or manufacturing use only, not for drug, food and household use.