




Current Data Parameters
NAME 0905-4963
EXPNO 10
PROCNO

F2 - Acquisition Parameters
Date_ 20240906
Time 14:07 h
INSTRUM spect
PROBHD zgpg30
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 128.07
DN 62.480 usec
DE 6.50 usec
TE 298.2 K
D1 1.00000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 14.6979995 W

F2 - Processing parameters
SF 400.1500922 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

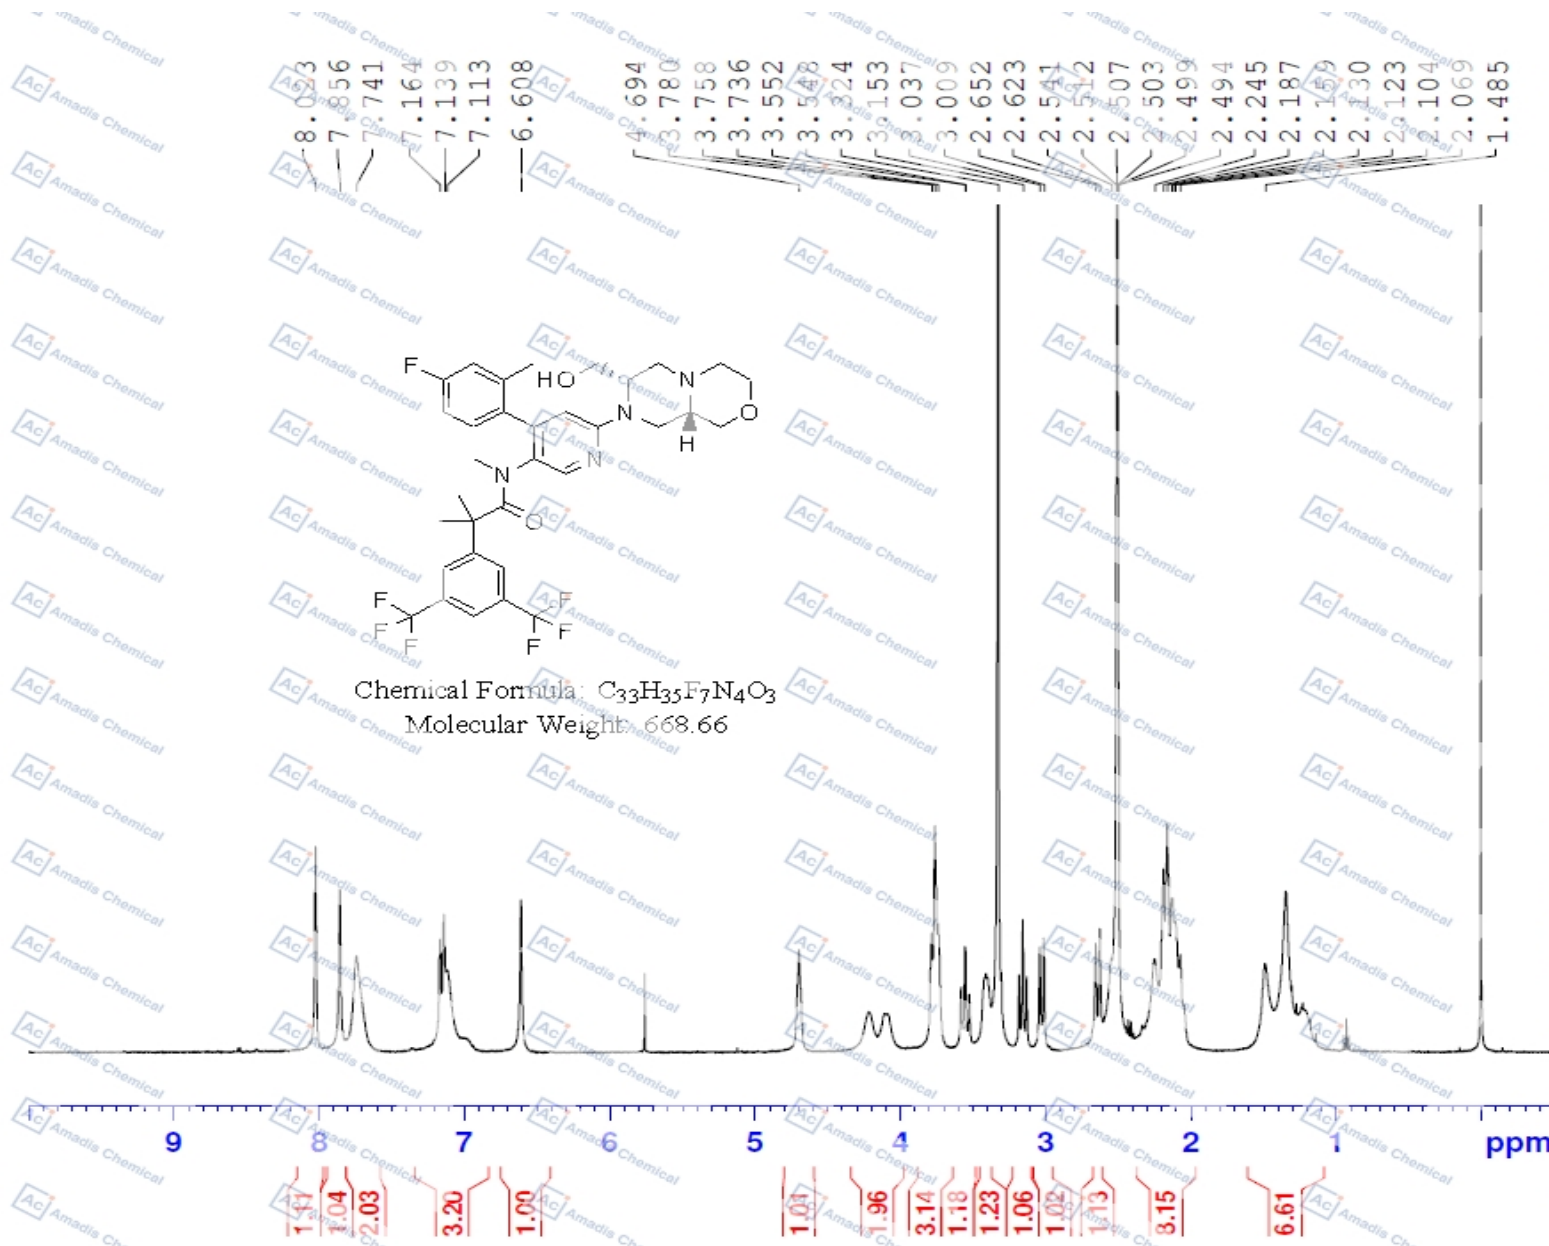

*For laboratory or manufacturing use only, not for drug, food and household use.