



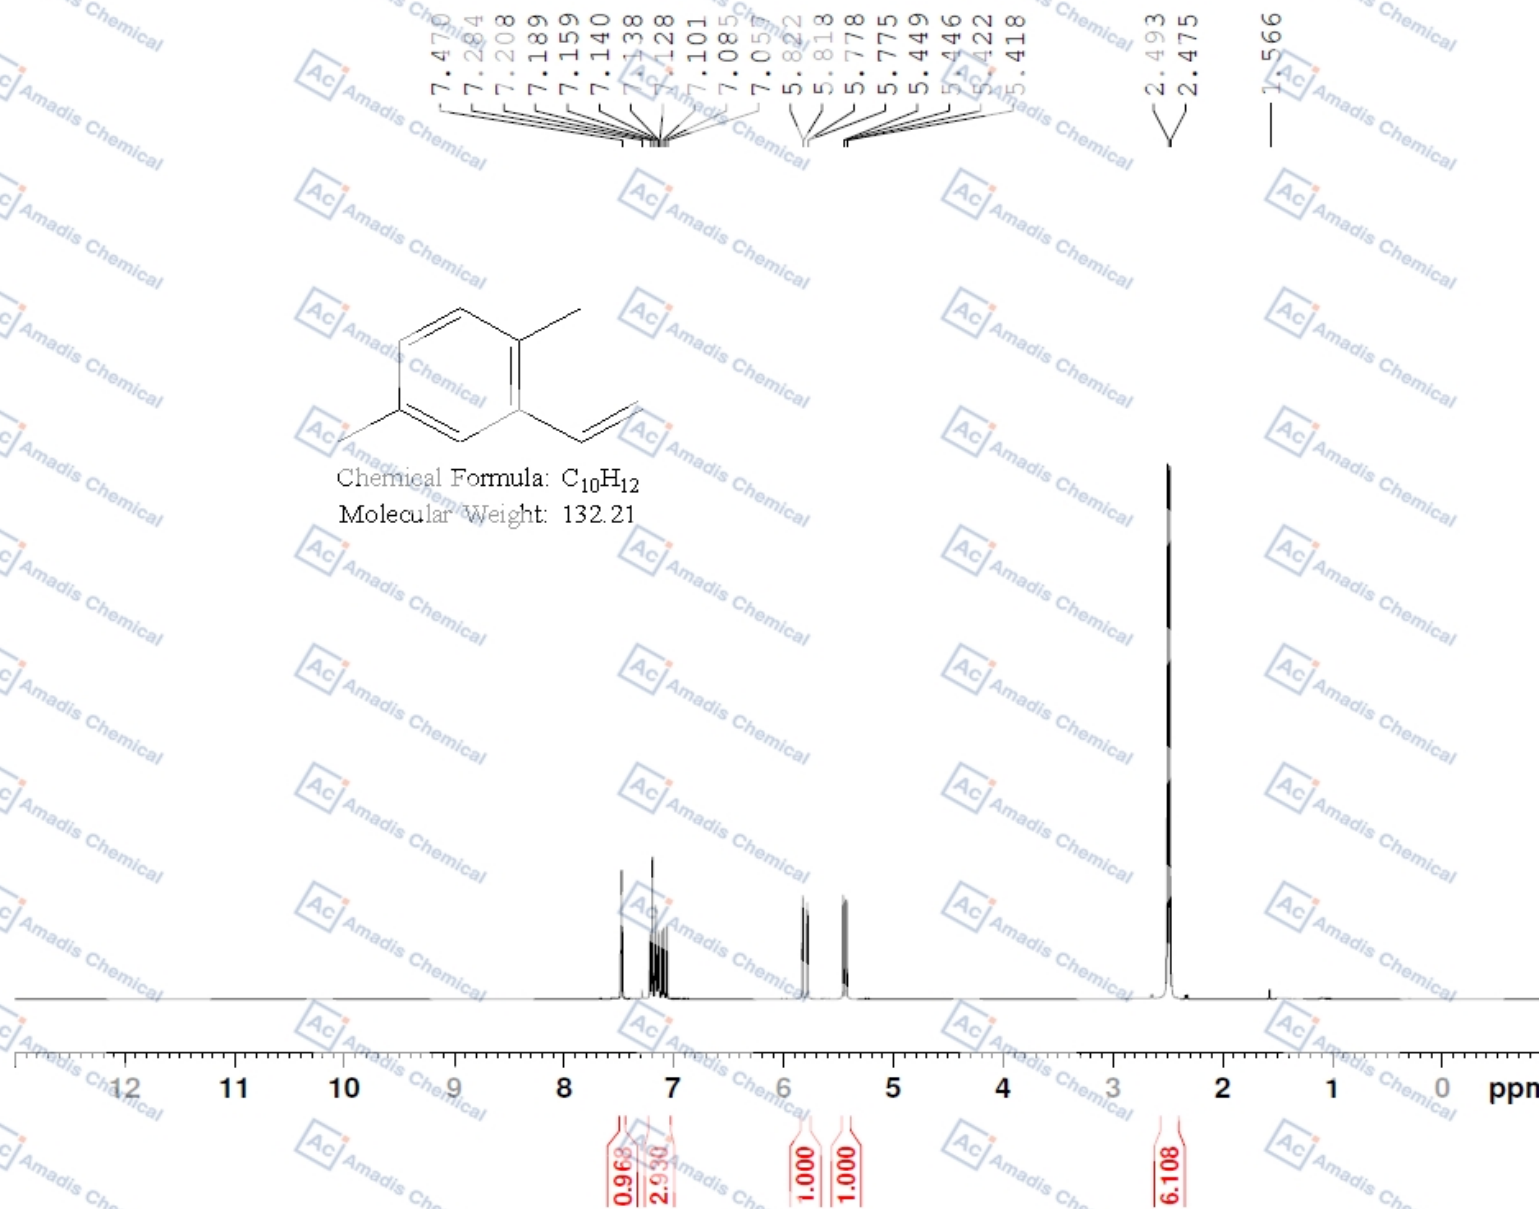

Current Data Parameters
NAME 2039-89-6P2535658
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230331
Time 18.35 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (zg30
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 16
DW 61.000 usec
DE 13.89 usec
TE 298.0 K
D0 1.00000000 sec
D1 1
SFO1 400.1324708 MHz
NUC1 1H
P0 2.67 usec
P1 8.00 usec
PL1 22.77899933 W

Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

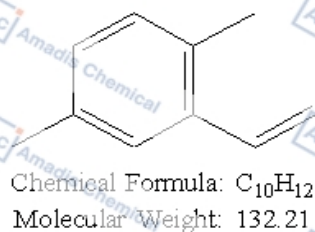

*For laboratory or manufacturing use only, not for drug, food and household use.