



MS of 2386432-28-4

Peak Analysis

Injection Details

Injection Name:	0321-5203	Run Time (min):	2.97
Vial Number:	RC3	Injection Volume:	2.00
Injection Type:	Unknown		
Calibration Level:			
Instrument Method:	MS-3MIN-MW-100-1500		
Processing Method:	Qualitative_20250311	Dilution Factor:	1.0000
Injection Date/Time:	25/Mar/25 15:00	Sample Weight:	1.0000

Mass Spectrum

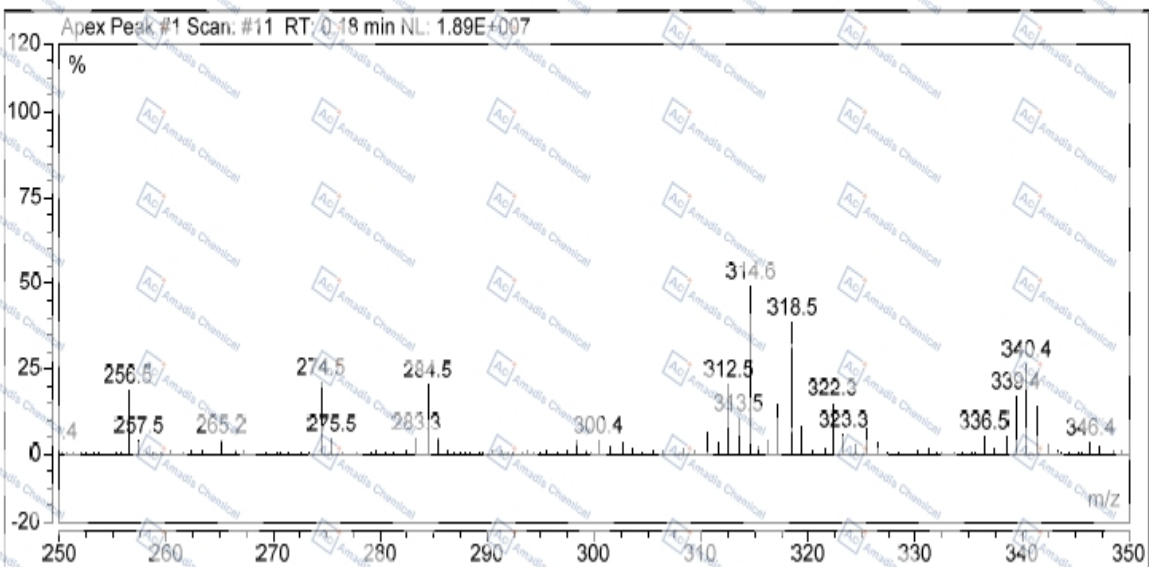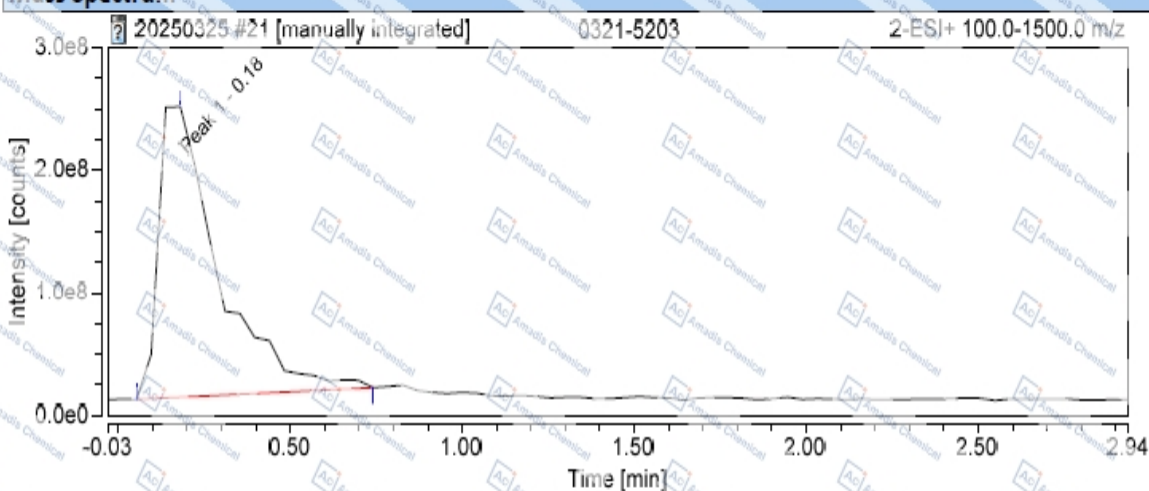

*For laboratory or manufacturing use only, not for drug, food and household use.

*If you have any comments and suggestions, please contact us by sales@amadischem.com