


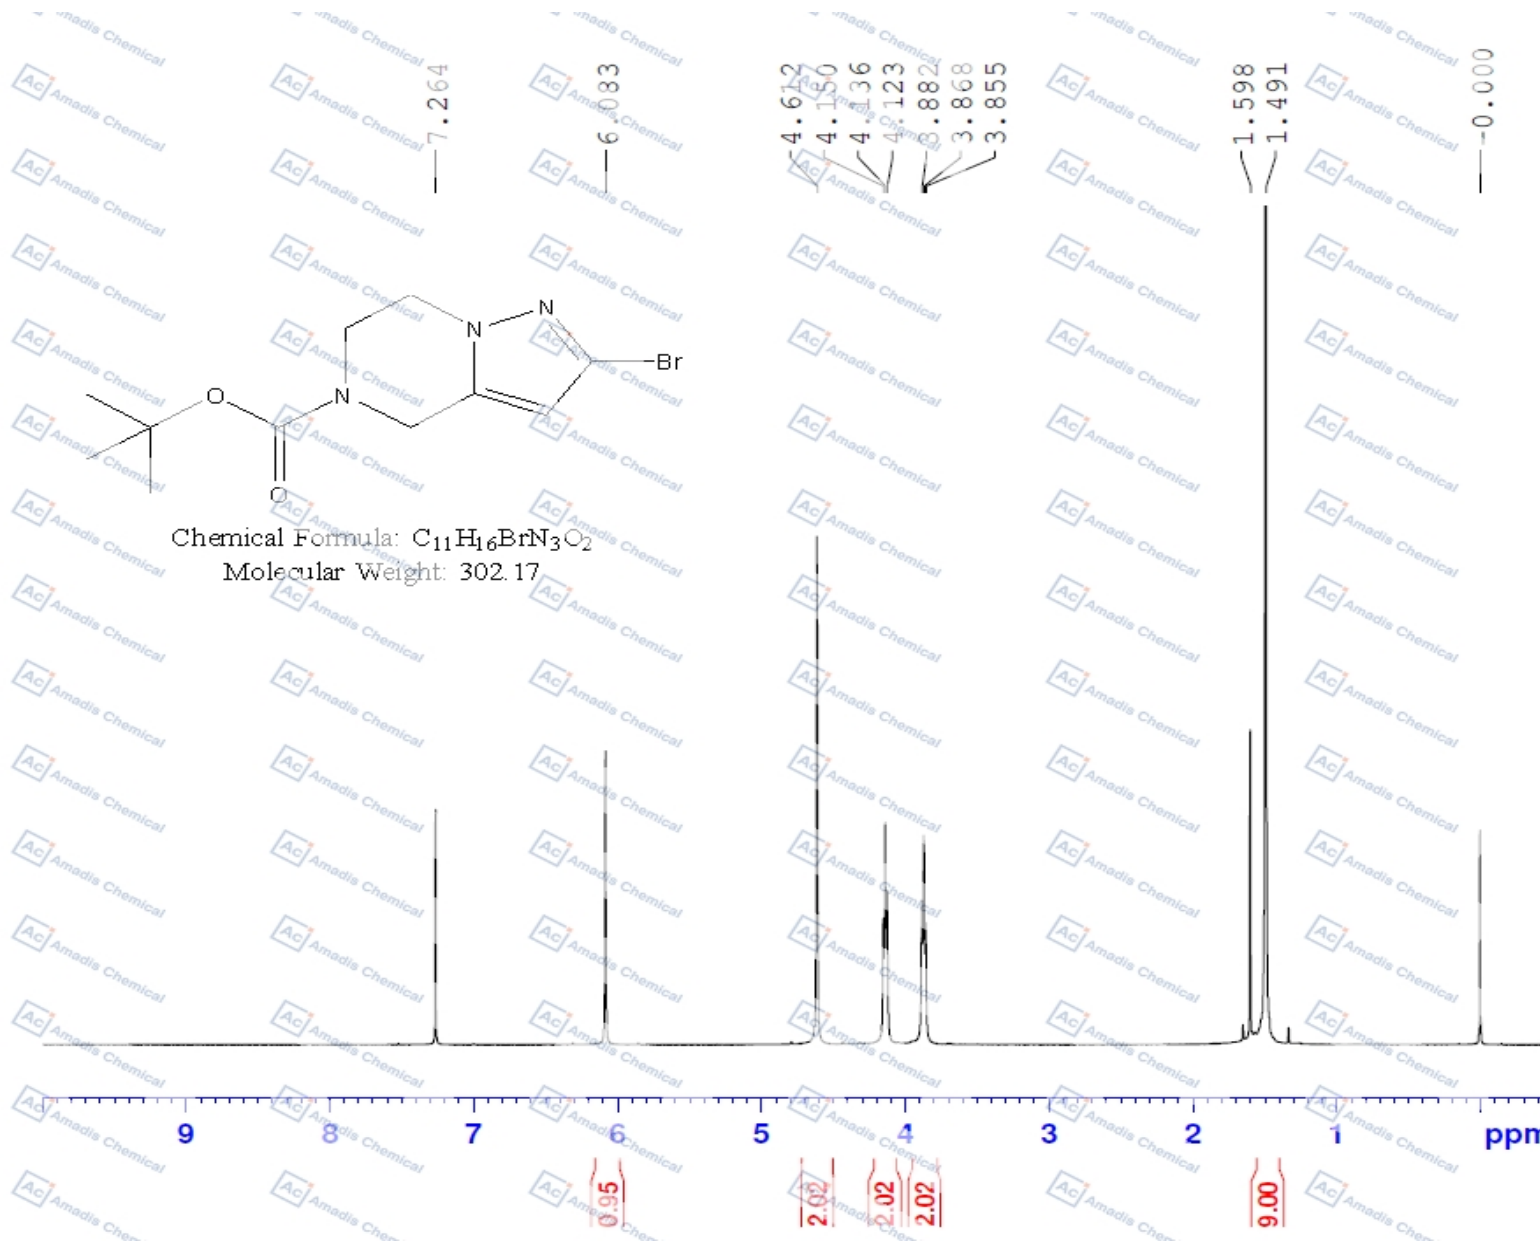

Current Data Parameters
NAME 1016-5015
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters

Date_ 20241031
Time 14:59
INSTRUM spect
PROBHD Z146098_0490 (1
PULPROG zgpg30
TD 65536
SOLVENT CDCl₃
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 1224.7
DW 62.400 usec
DE 6.50 usec
TE 298.3 K
D1 1.00000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
PL 10.90 usec
PLW 14.6979955 W

F2 - Processing parameters

SI 65536
SF 400.1500822 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.