


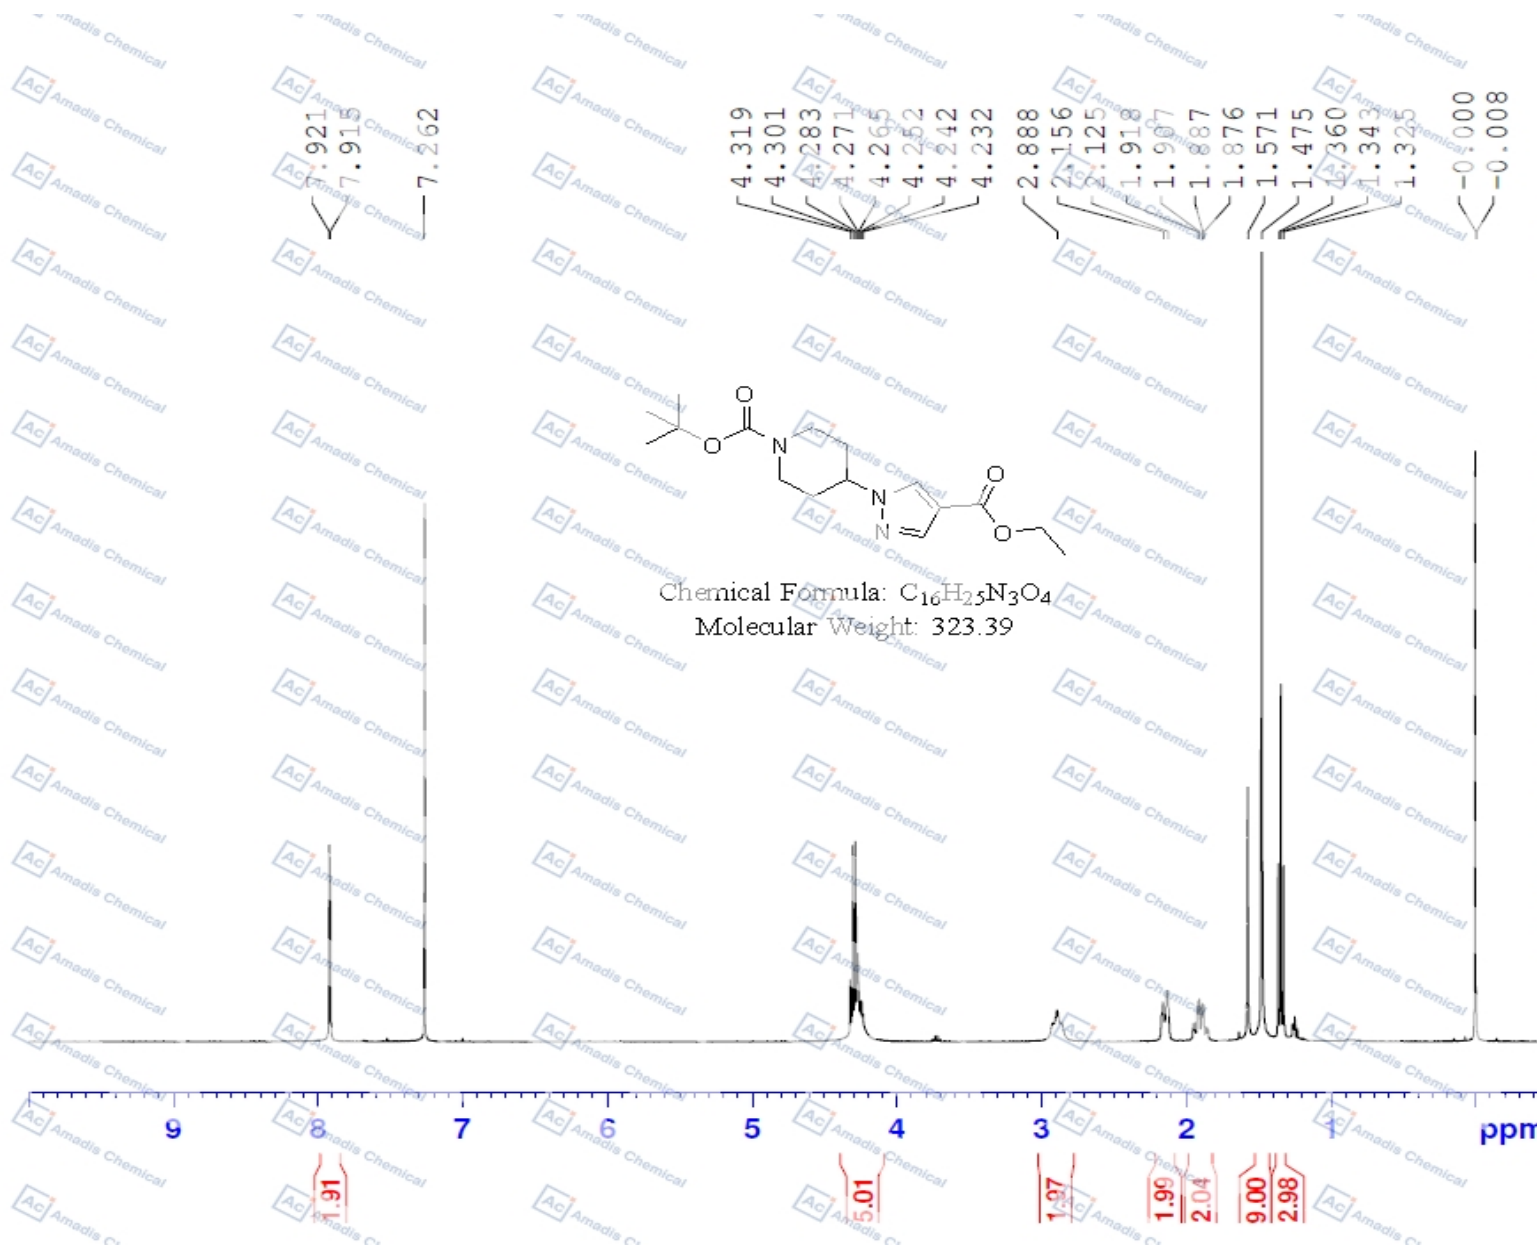

BRUKER

Current Data Parameters	
NAME	0529-5315
EXPNO	10
PROCNO	1

F2 - Acquisition Parameters	
Date_	20250603
Time	14:44 h
INSTRUM	spect
PROBHD	116098_0490 (
PULPROG	zg30
TD	65536
SOLVENT	CDCl ₃
NS	16
DS	2
SWH	8012.840 Hz
FIDRES	0.244537 Hz
AQ	4.0894465 sec
RG	123.07
DW	62.400 usec
DE	6.50 usec
TE	298.0 K
D1	1.00000000 sec
TD0	65536
SFO1	400.1524709 MHz
NUC1	1H
P1	10.00 usec
PL1	15.59300241 W

F2 - Processing parameters	
SI	65536
SF	400.1500289 MHz
WDW	EM
SSB	0
LB	0.30 Hz
GB	0
PC	1.00

*For laboratory or manufacturing use only, not for drug, food and household use.