


MS of 2387505-73-7

MASS SPECTROMETRY REPORT

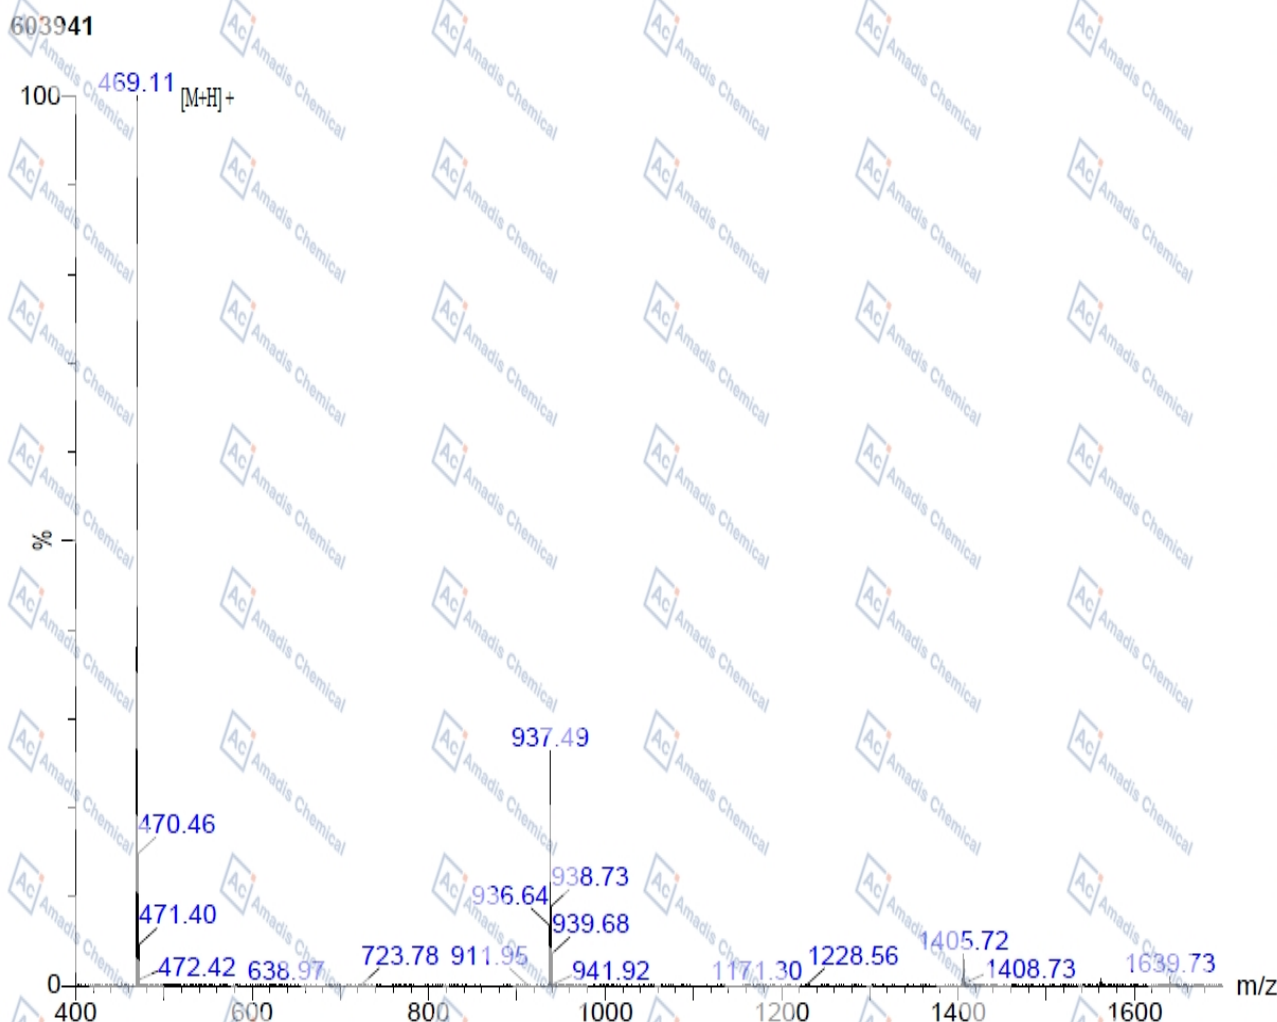

Sample Description

Analyzed date: 2022-12-20

Analyst: SHAO

Sample: 603941

M.W.: 468.6

Lot. No.:

Instrument

Waters 2695

Probe:

ESI

Nebulizer Gas Flow:

1.5L/min

CDL:

-20.0v

CDL Temp.:

250 °C

Block Temp:

200 °C

Probe Bias:

+4.5kv

Detector:

1.5kv

T. Flow:

0.5ml/min

B. Conc.:

50%H₂O/50%ACN

***For laboratory or manufacturing use only, not for drug, food and household use.**

**if you have any comments and suggestions, please contact us by sales@amadischem.com*