


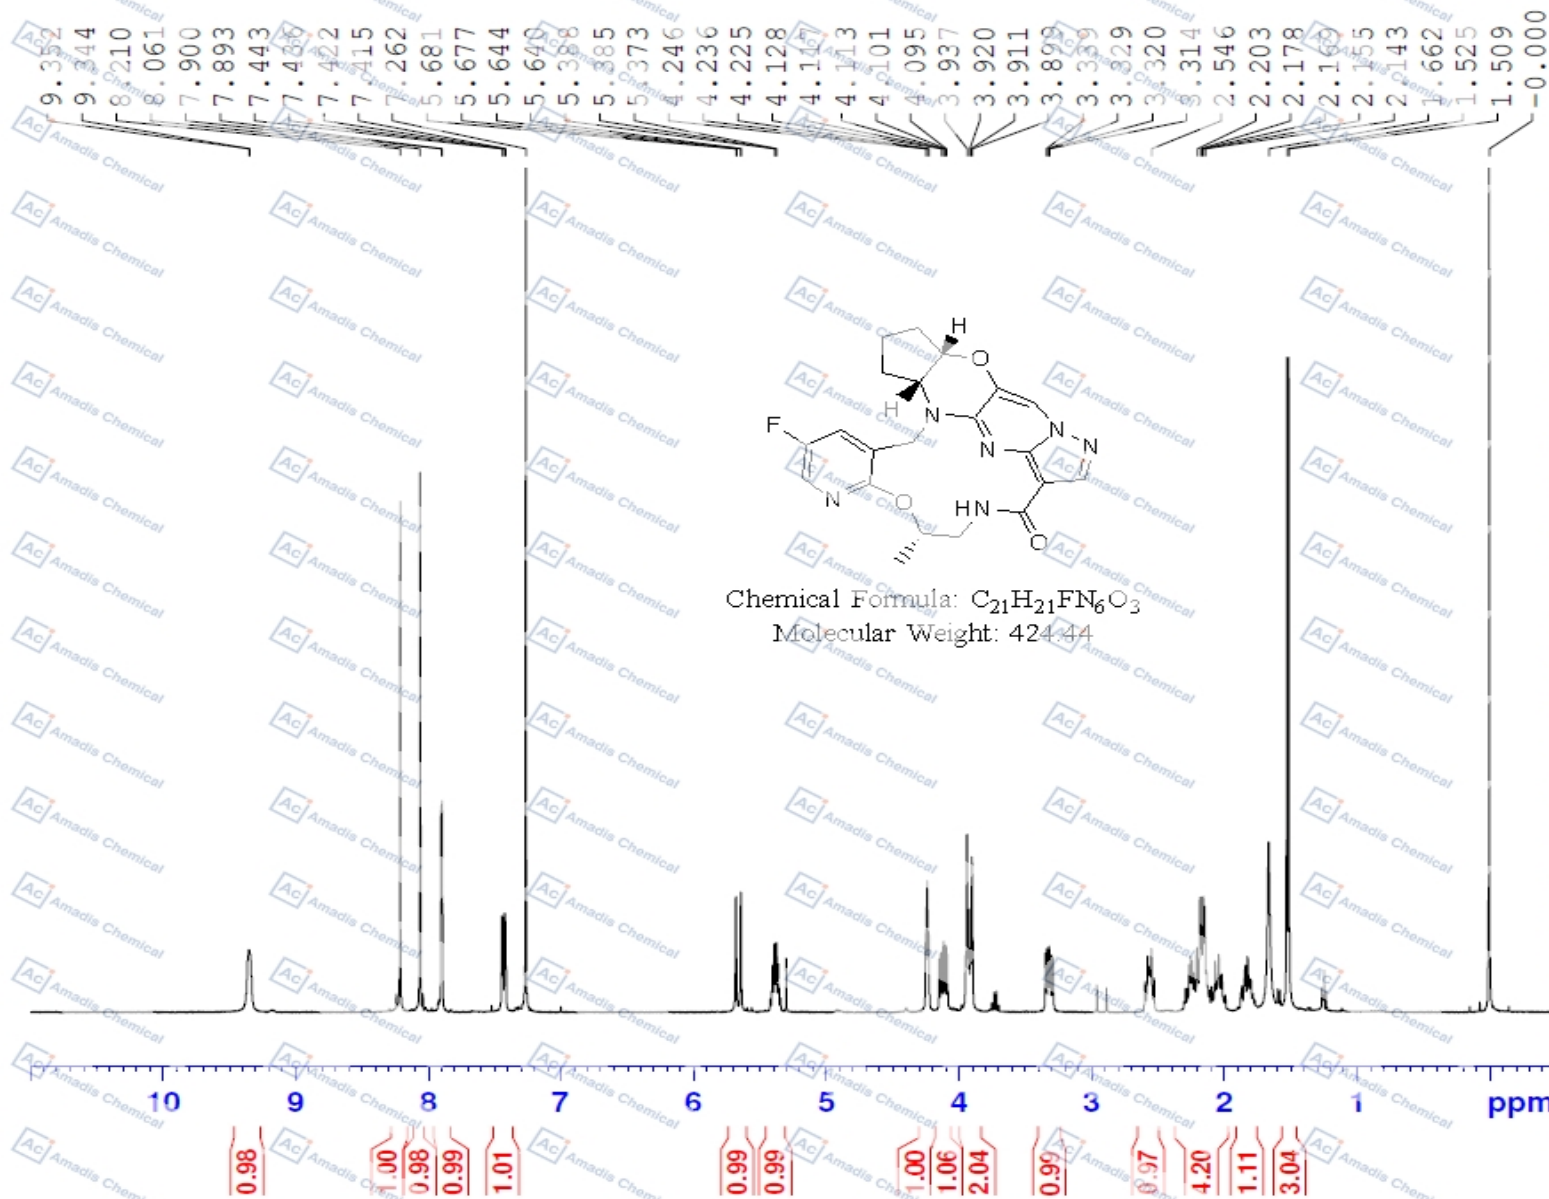

Current Data Parameters
NAME 0616-2330
EXPNO 1
PROCNO 1

Acquisition Parameters
Date_ 20250817
Time 12.21
INSTRUM spect
PROBHD z116098_0499 (400 MHz 1H NMR)
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.089465 sec
RG 1232.00
DW 62.400 usec
DE 6.50 usec
TE 299.3 K
F1C 1.0000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 15.59300041 W

F2 - Processing parameters
SI 32768
SF 400.1500089 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.