


MS of 60748-45-0

MASS SPECTROMETRY REPORT

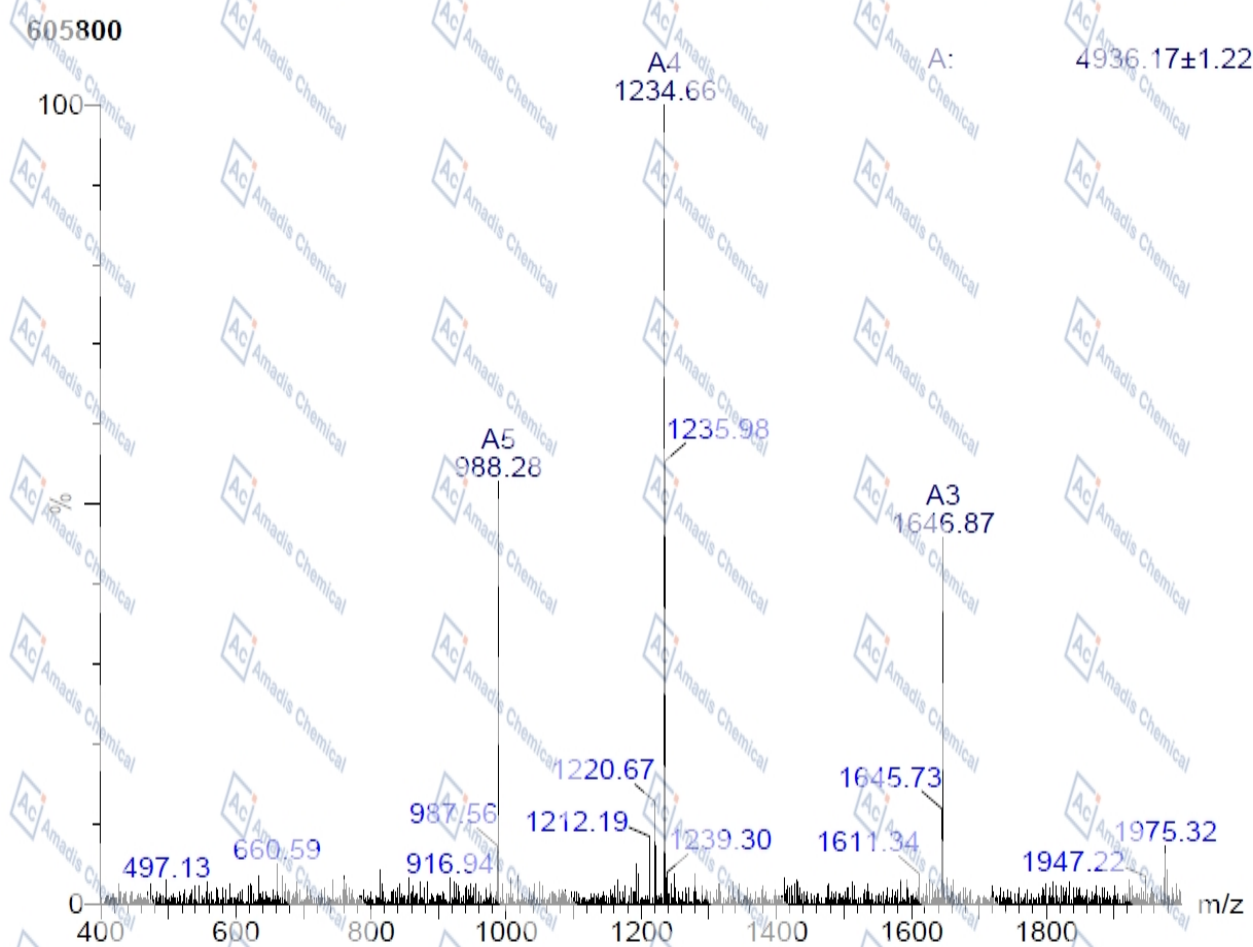

Sample Description

Analyzed date: 2024-06-11

Analyst: SHAO

Sample: 605890

M.W.: 4934.7

Lot No.:

Instrument

Waters 2695

Probe:

ESI

Probe Bias:

4.5kv

Nebulizer Gas Flow:

1.5L/min

Detector:

1.5kv

CDL:

-20.0v

T. Flow:

0.5ml/min

CDL Temp.:

250 °C

B. Conc.:

50% H₂O/50% ACN

Block Temp.:

200 °C

***For laboratory or manufacturing use only, not for drug, food and household use.**

**if you have any comments and suggestions, please contact us by sales@amadischem.com*