



LCMS of 788824-64-6

File: D:\data\1\Data\外测数据\MJ-549-B-5 (1) 2024-12-18 14-23-41.D
Injection Date : 18 Dec 24 2:24 pm +0800 Tgt Mass (ZXX) :
Sample Name : MJ-549-B-5 Location :
Acq. Operator : 系统 Inj : 1
Spec. Reported : MS Integration Inj Volume : 5 ul
Acq. Method : D:\data\1\Methods\LCMS NH4FA 8min 210-254nm.M
Analysis Method : D:\data\1\Methods\clean column 60min.M
Sample Info : 色谱柱: ID: 005, Waters Xbridge C18, 4.6*100mm, 3.5um
Method Info :

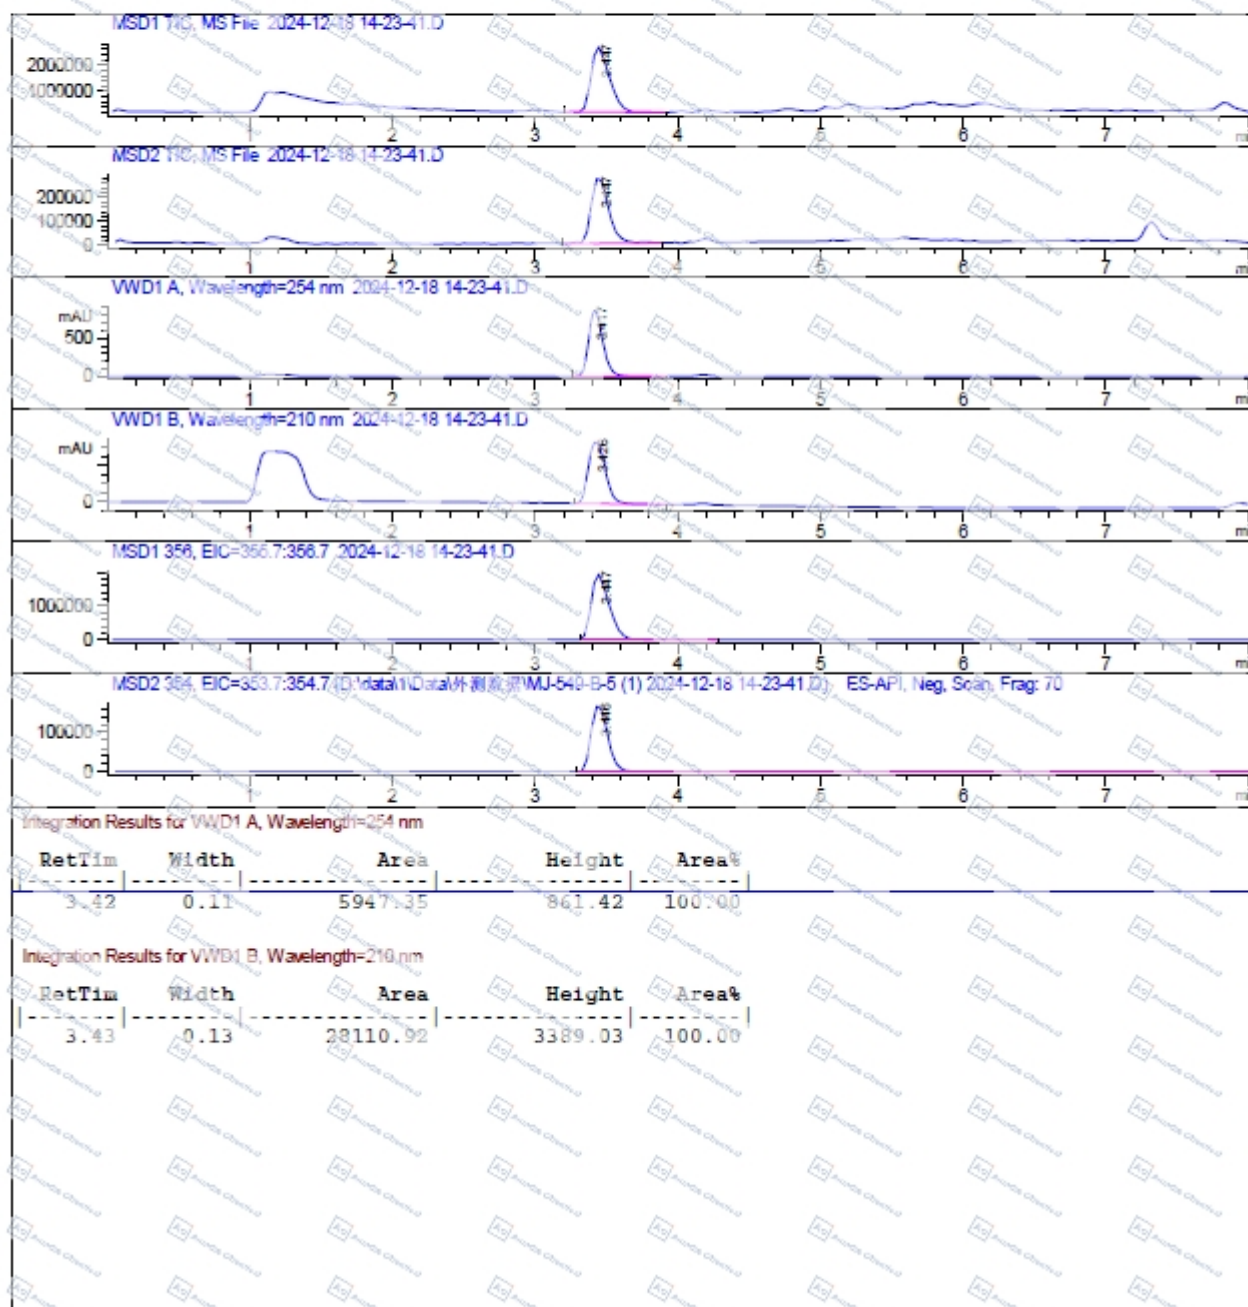


Ret. Time: 3.45 <<<< POSITIVE SPECTRA >>>>

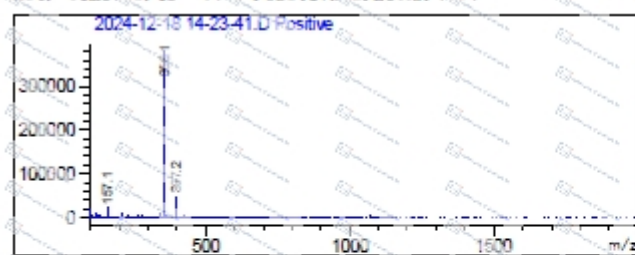


Base Peak Ion Ratios:				2nd Largest Peak Ion Ratios:			
Ion	Mass	Abundance	Ratio	Ion	Mass	Abundance	Ratio
A	356.10	279269	100.00	B	397.20	46641	100.00
A + 1	357.10	56558	14.51	B + 1	398.15	7730	16.57
A + 2	358.10	6458	1.70	B + 2	399.15	1206	2.62
A + 3	359.15	858	0.04	B + 3	400.15	76	0.16
A + 4	360.00	68	0.02	B + 4	401.25	215	0.45
A + 5	361.00	357	0.04	B + 5	402.15	72	0.15

Ret. Time: 3.45 <<<< NEGATIVE SPECTRA >>>>

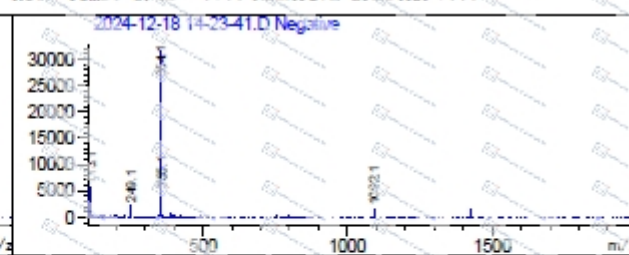


Base Peak Ion Ratios:				2nd Largest Peak Ion Ratios:			
Ion	Mass	Abundance	Ratio	Ion	Mass	Abundance	Ratio
A	356.10	11377	100.00	B	312.10	6728	100.00
A + 1	357.15	4022	35.37	B + 1	314.10	121	3.35
A + 2	356.10	464	1.43				
A + 3	357.05	53	0.37				

Ret. Time: 3.45 <<<< POSITIVE SPECTRA >>>>

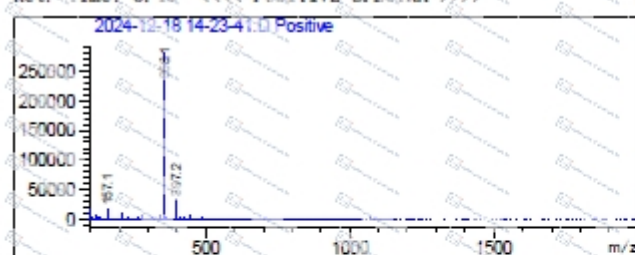

Base Peak Ion Ratios:				2nd Largest Peak Ion Ratios:			
Ion	Mass	Abundance	Ratio	Ion	Mass	Abundance	Ratio
A	356.10	278972	100.00	B	397.20	34288	100.00
A + 1	357.10	41306	14.83	B + 1	398.15	6919	20.18
A + 2	358.10	4759	1.71	B + 2	399.15	1193	3.48
A + 3	359.20	358	0.05	B + 3	400.20	115	0.34
A + 4	360.06	127	0.07	B + 4	401.25	167	0.49
A + 5	361.15	565	0.20	B + 5	402.15	53	0.15

Ret. Time: 3.45 <<<< NEGATIVE SPECTRA >>>>

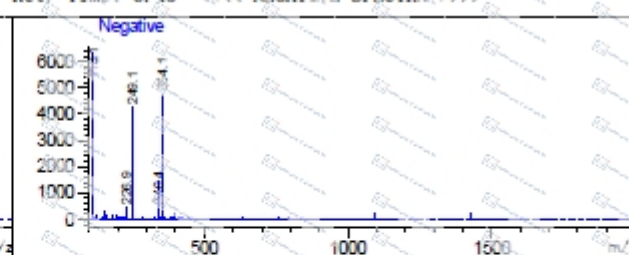

Base Peak Ion Ratios:				2nd Largest Peak Ion Ratios:			
Ion	Mass	Abundance	Ratio	Ion	Mass	Abundance	Ratio
A	113.10	6279	100.00	B	356.10	4763	100.00
A + 1	114.10	95	1.51	B + 1	357.15	701	15.35
A + 2	114.90	2	0.03	B + 2	356.10	71	1.50
A + 5	119.10	1	0.02	B + 3	357.05	9	0.17
				B + 4	358.00	2	0.04
				B + 5	359.15	3	0.07

*For laboratory or manufacturing use only, not for drug, food and household use.

*If you have any comments and suggestions, please contact us by sales@amadischem.com