


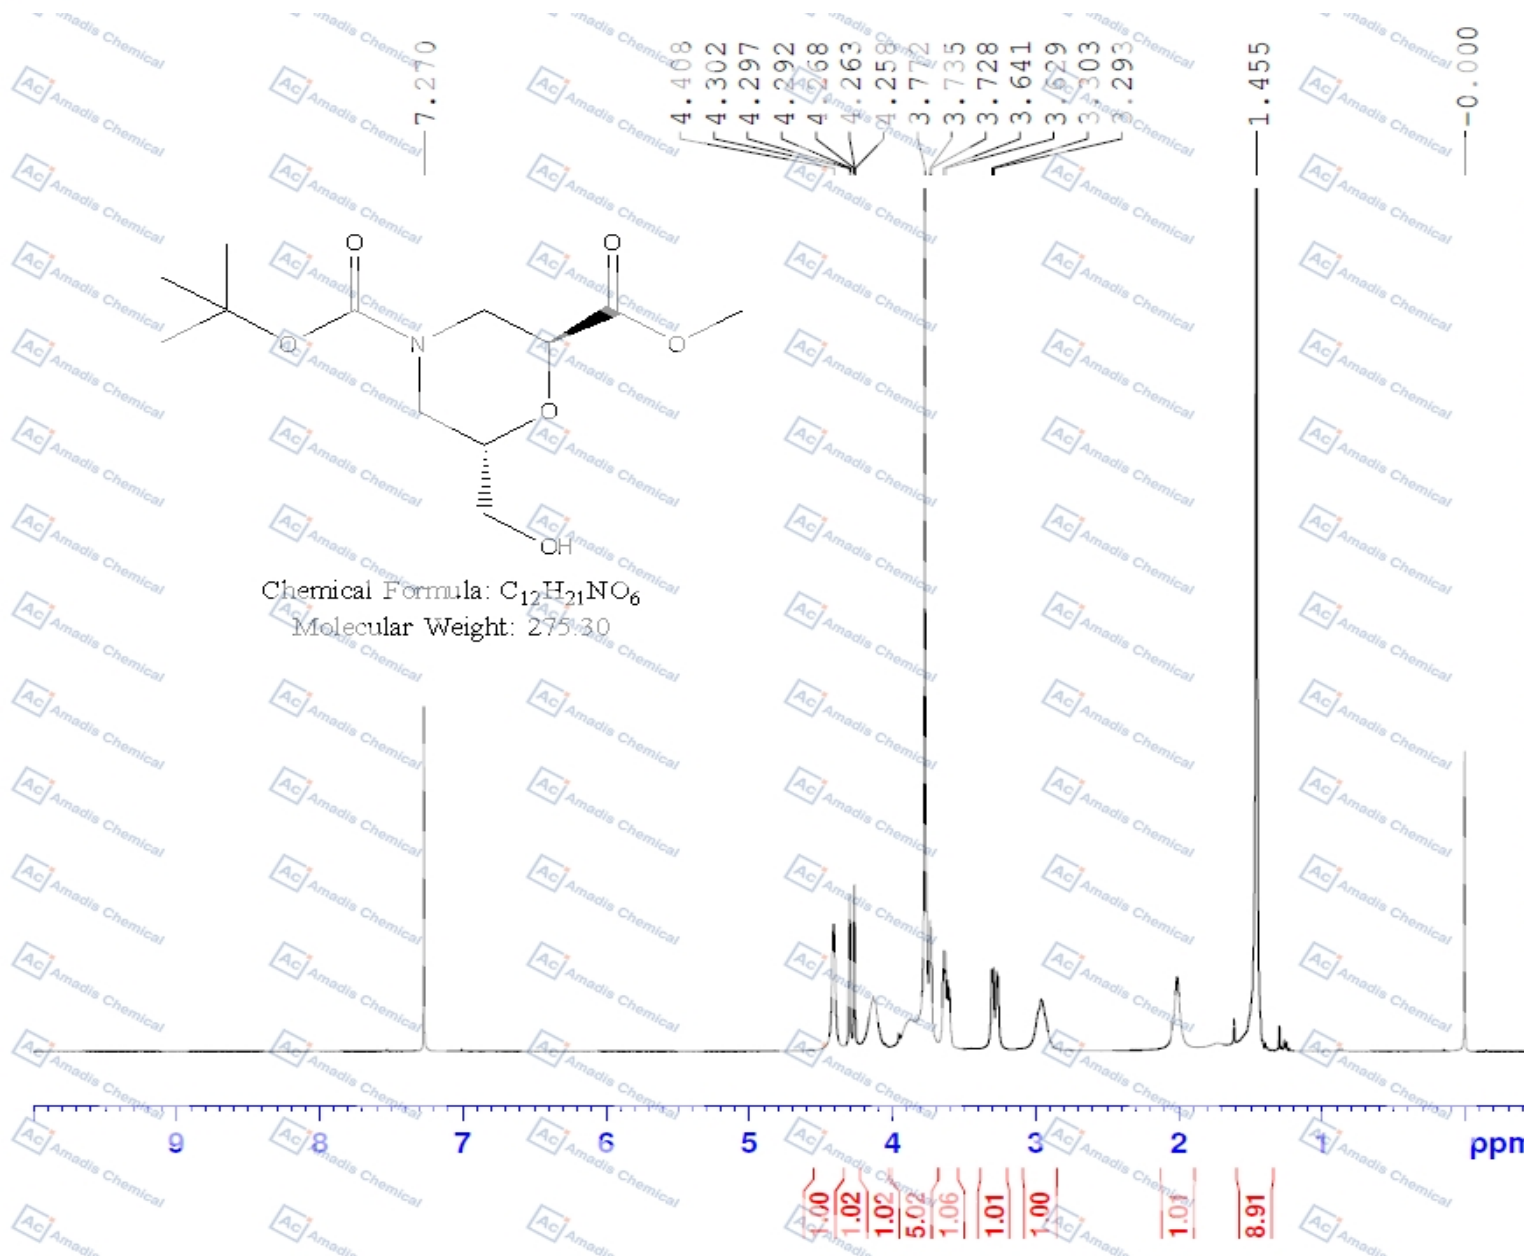

Current Data Parameters
NAME 1007-5109
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250108
Time 15:02 h
INSTRUM spect
PROBHD zg30
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 8012.679 Hz
FIDRES 0.244537 Hz
AQ 4.0894465 sec
RG 79.19
DW 62.400 usec
DE 6.50 usec
TE 295.7 K
D1 1.00000000 sec
TDC 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PI1 15.59300081 W

F2 - Processing parameters
SI 65536
SF 400.1500958 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.60

*For laboratory or manufacturing use only, not for drug, food and household use.