


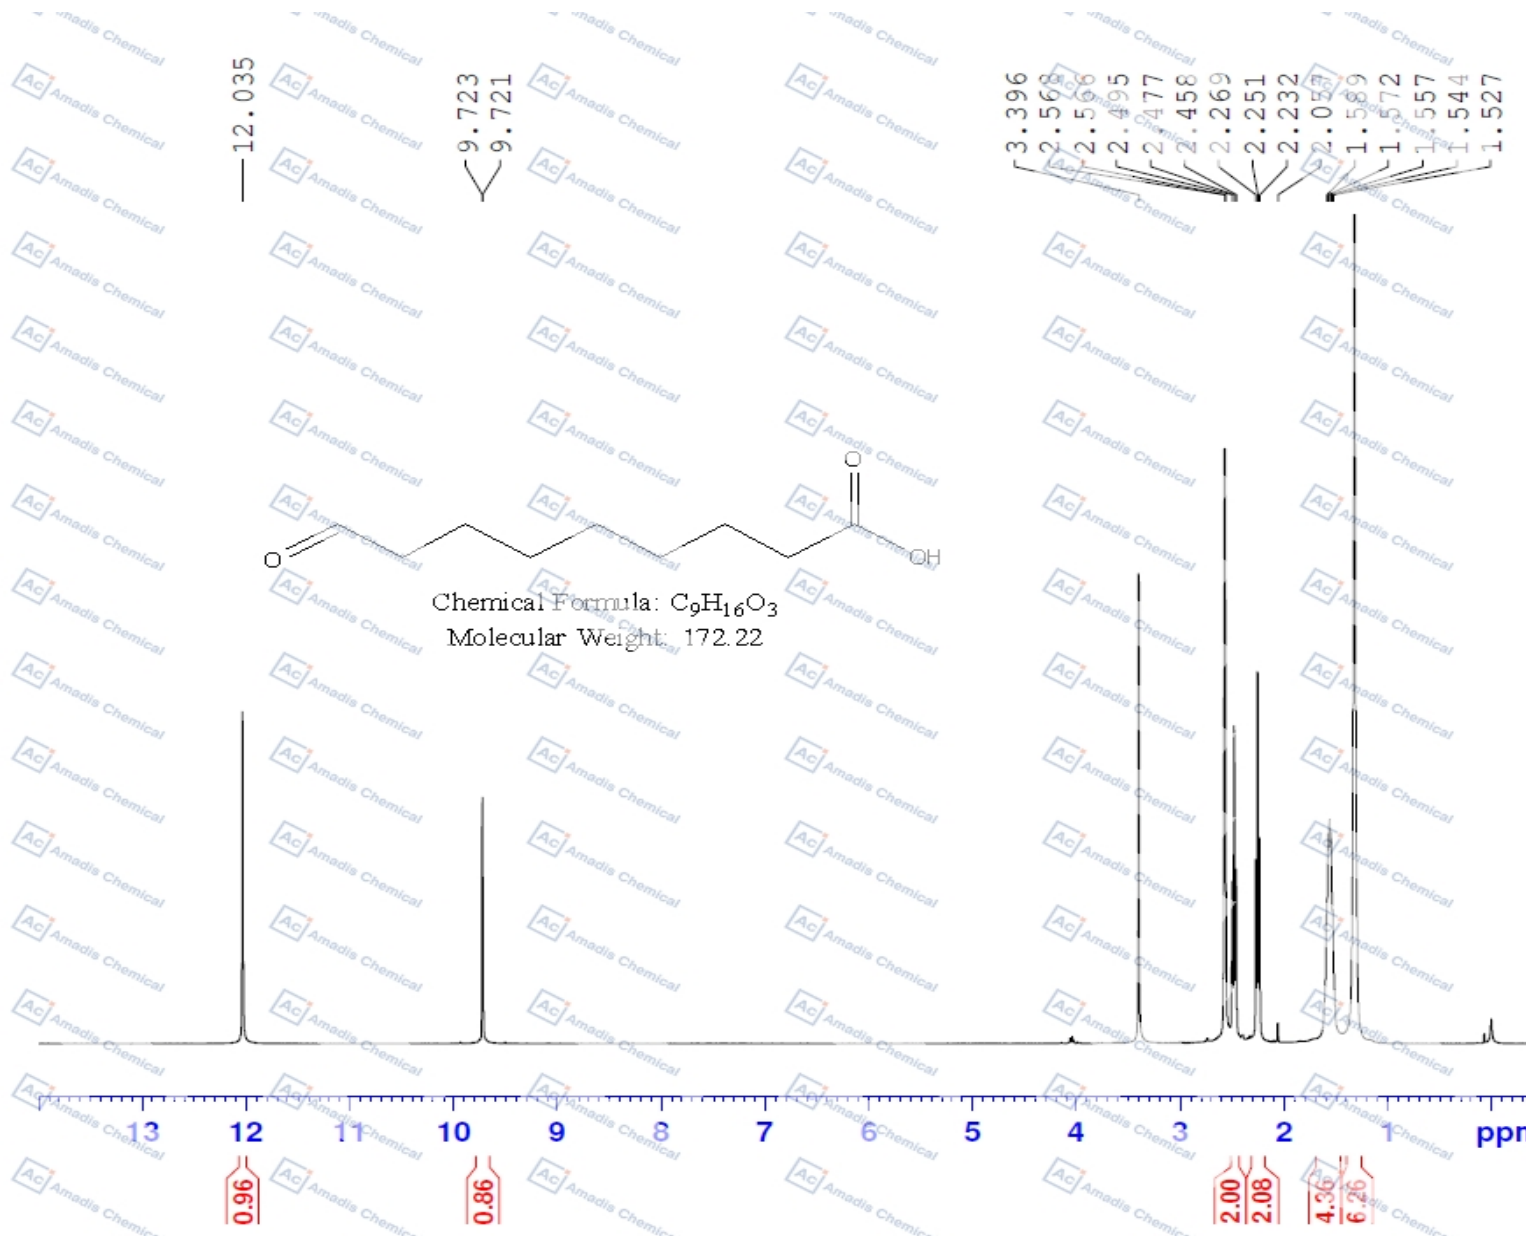

Current Data Parameters
NAME 0314-5178
EXTNO 1
PROCNO 1

F2 - Acquisition Parameters

DATE 20250317
Time 15.58 H
INSTRUM spect
PROBHD z116098_0490
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 4
SWH 8012.820 MHz
FIDRES 0.244532 Hz
AQ 4.089465 sec
RG 98.69
DW 62.400 usec
DE 6.50 usec
TE 296.2 K
D1 1.00000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.460 usec
PLW1 15.59300041 W

F2 - Processing parameters

SI 65536
SF 400.1499766 MHz
WDW EM
SSB 0
LB 0.430 Hz
GB
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.