




Current Data Parameters  
NAME 0522-5284  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters

DATE\_ 20250523  
Time 10.47 W  
INSTRUM spect  
PROBHD ztt6098\_0490 (1  
PULPROG zgpg30  
TD 65536  
SOLVENT DMSO  
NS 16  
DE 123.407  
SWH 8012.820 Hz  
FIDRES 0.244532 Hz  
AQ 4.0894455 sec  
RG 123.407  
DW 62.400 usec  
DE 6.50 usec  
TE 298.4 K  
D1 1.00000000 sec  
TDO 1  
SFO1 400.1524709 MHz  
NUC1 1H  
P1 10.40 usec  
PLW1 15.59300041 W

F2 - Processing parameters

SI 65536  
SF 400.1500025 MHz  
WDW EM  
SSB 0  
LB 0.20 Hz  
GB 0  
PC 1.00

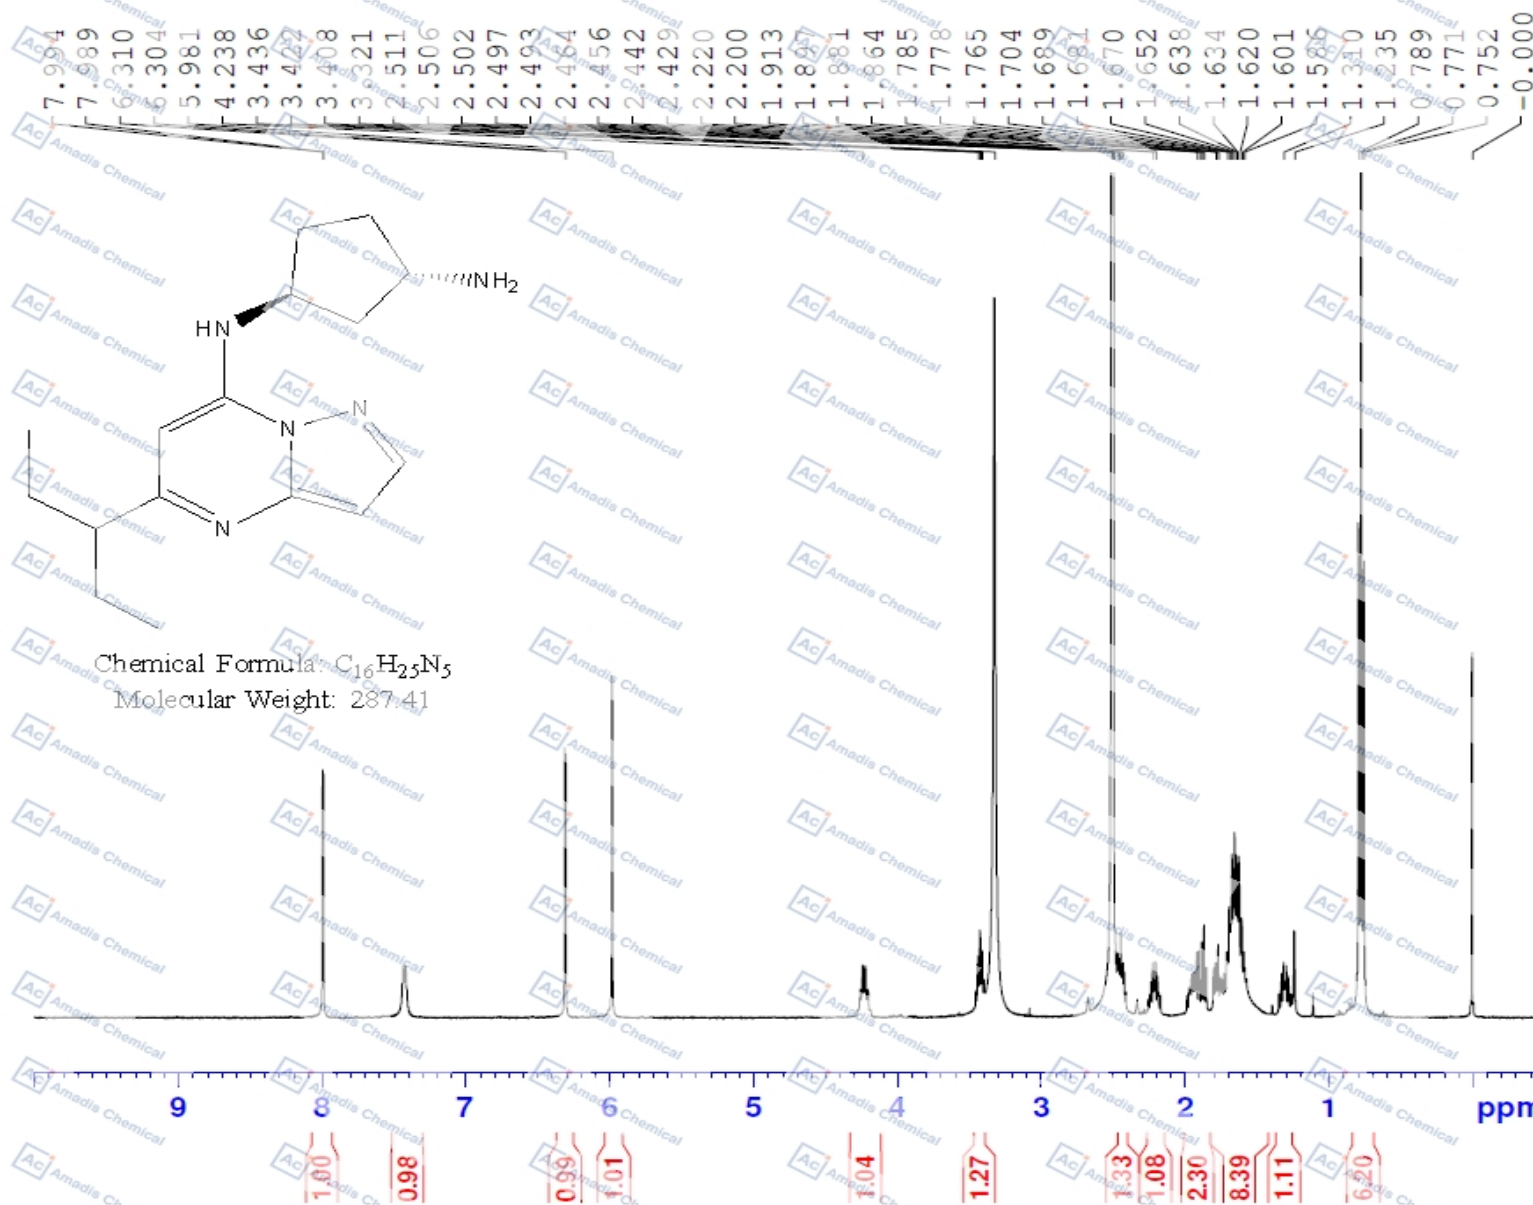

\*For laboratory or manufacturing use only, not for drug, food and household use.