



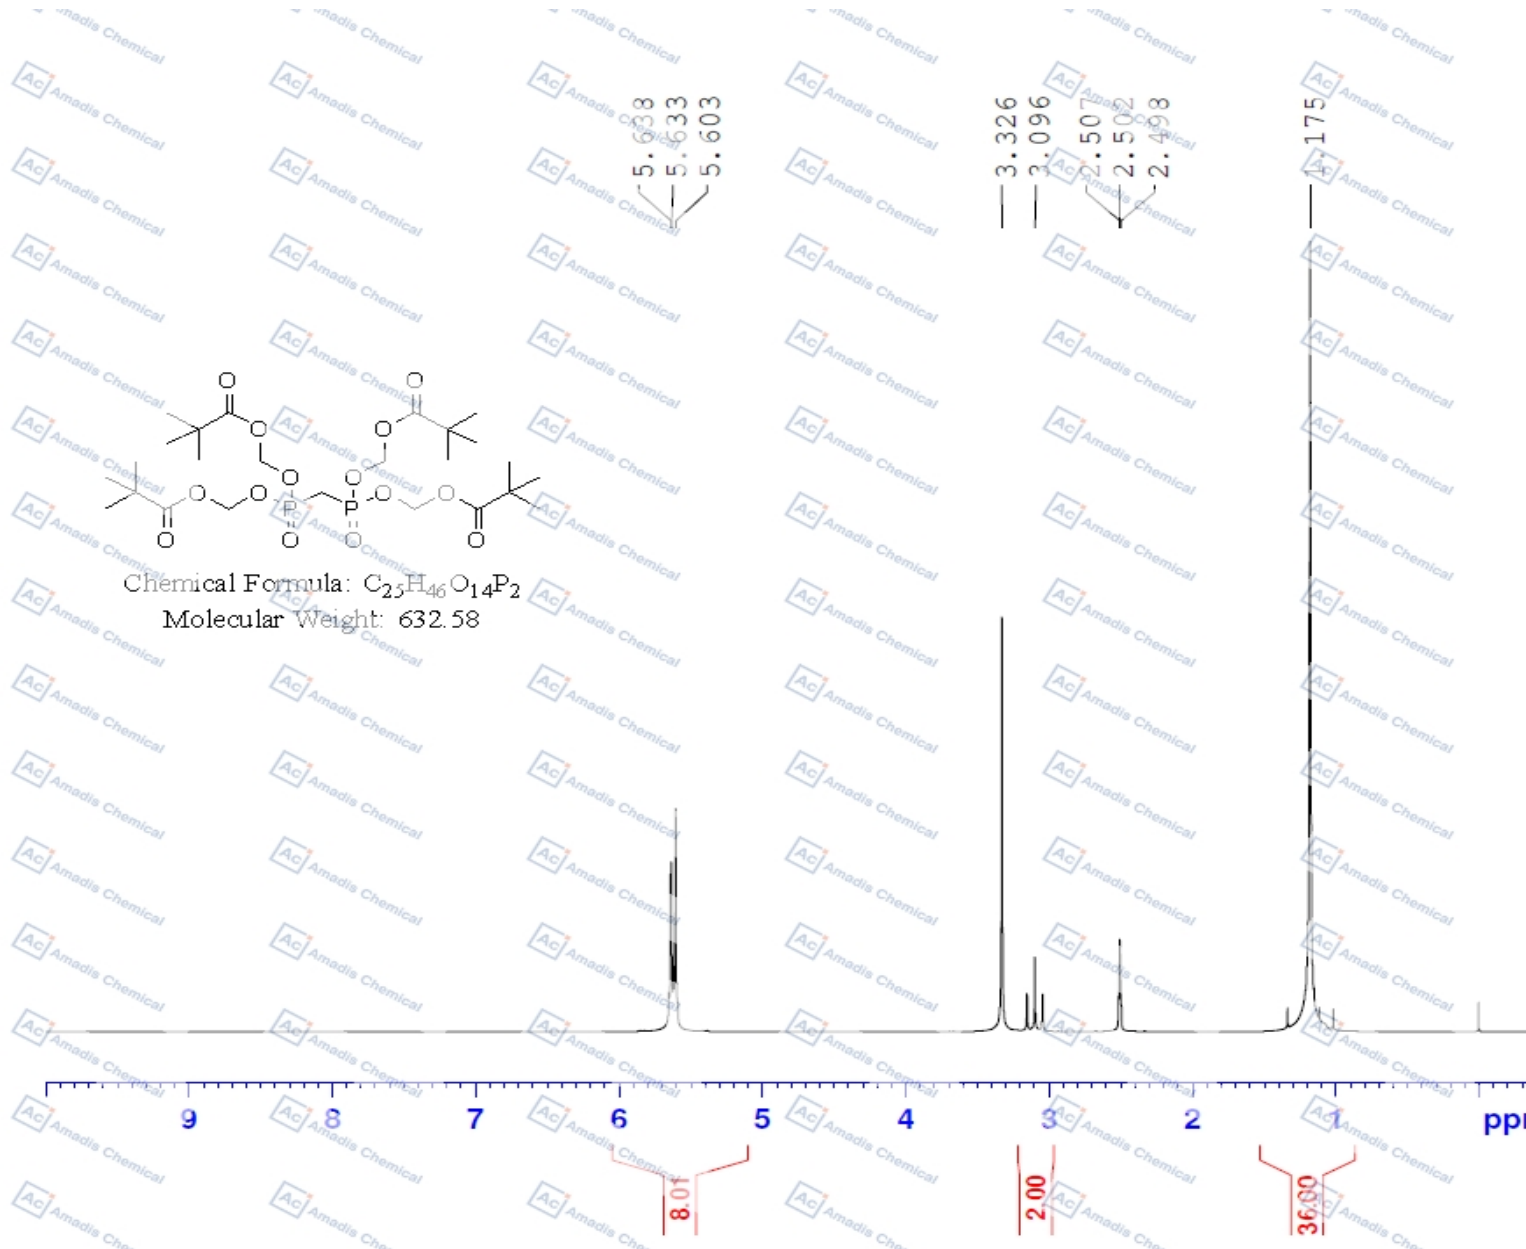

Current Data Parameters
NAME 0623-5341
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250624
Time 16:00 h
INSTRUM spect
PROBHD Z116098_0490 (4
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 67.79
DM 62.490 usec
DE 6.50 usec
TE 298.2 K
D1 1.00000000 sec
TDO 1
SFO 400.152409 MHz
NUC1 1H
P1 10.00 usec
PL1 15.59300641 W

F2 - Processing parameters
SI 65536
SF 400.150023 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

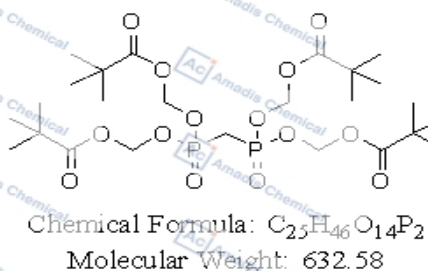

*For laboratory or manufacturing use only, not for drug, food and household use.