



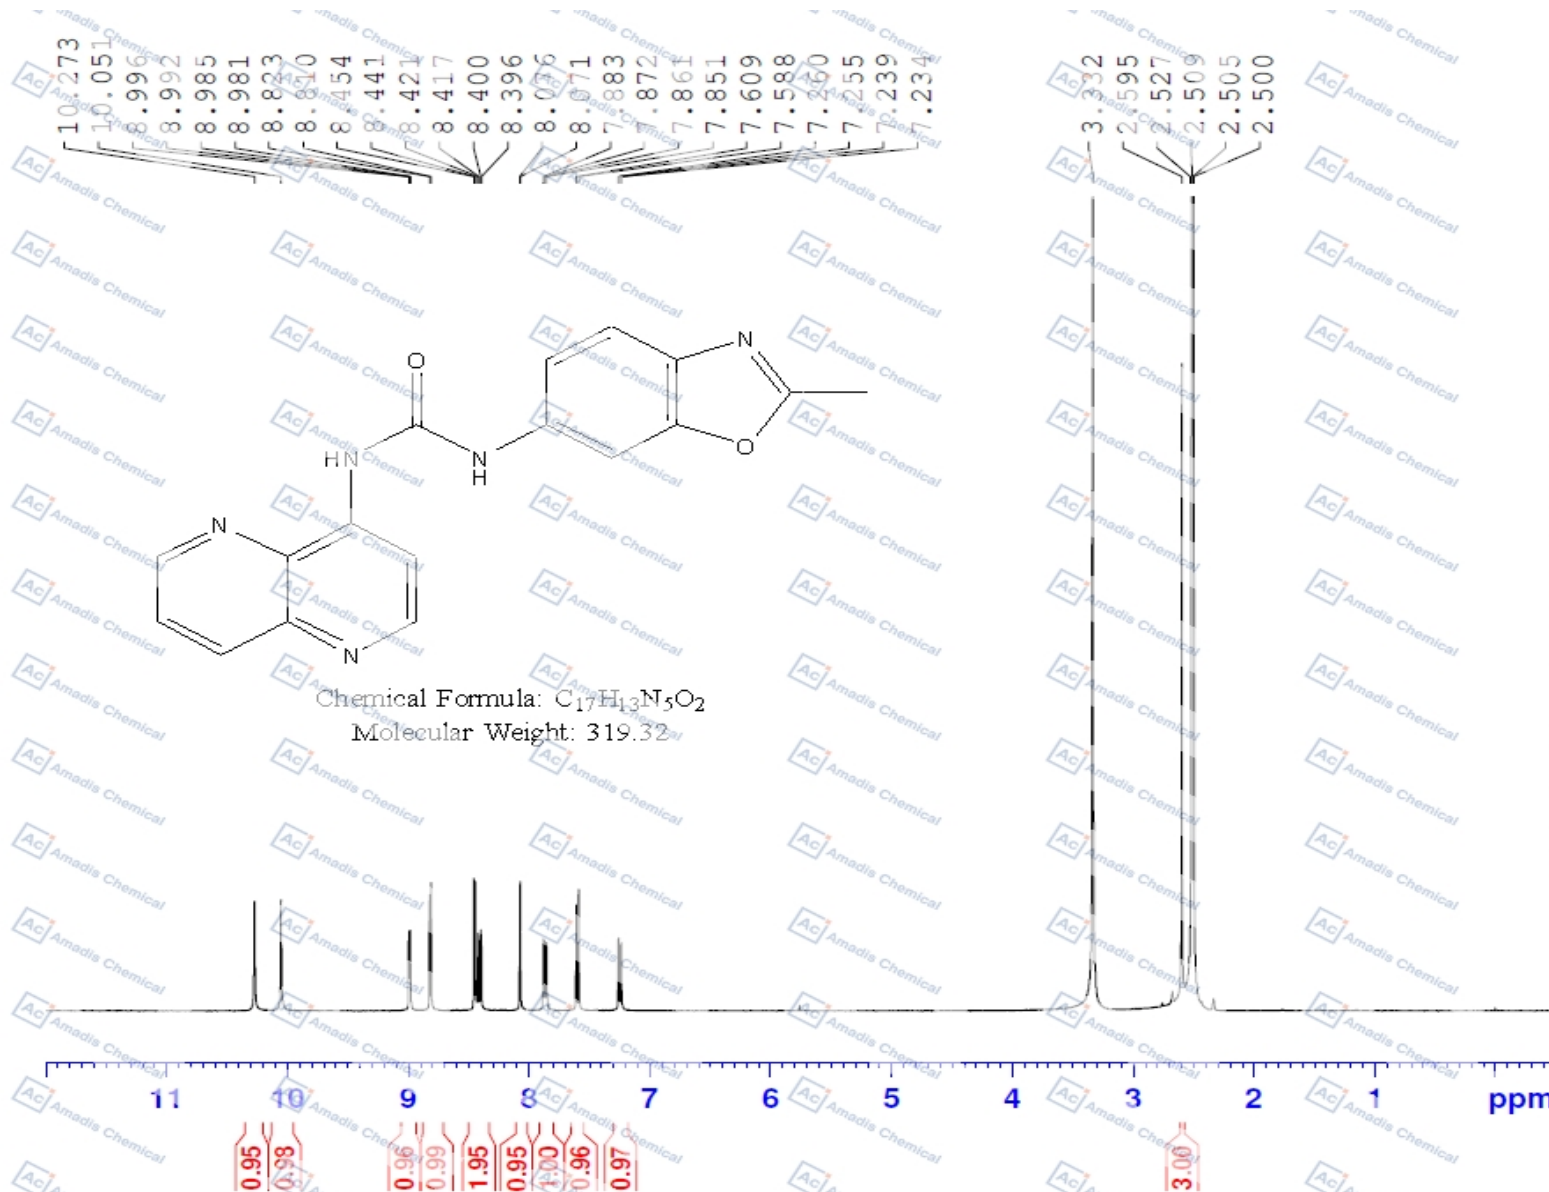

Current Data Parameters
NAME 1121-5065
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20241122
Time 14:59 h
INSTRUM spect
PROBHD Z116098_0490
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.890 Hz
FIDRES 0.244589 Hz
AQ 4.0894465 sec
RG 111.92
DQ 62.780 usec
DE 6.550 usec
TE 298.0 K
D1 1.00000000 sec
TDS 1
SFO1 400.1524039 MHz
NUC1 1H
P1 10.00 usec
PRW1 14.69799995 W

F2 - Processing parameters
SI 65536
SF 400.1500817 MHz
WDW Ac2M
SSB 0
LB 0.30 Hz
GB 0
PC 4.00

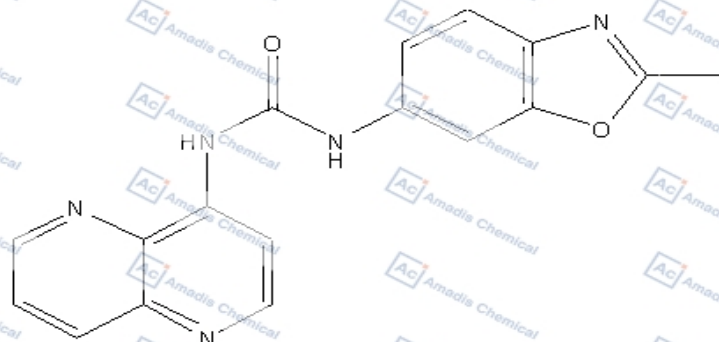

*For laboratory or manufacturing use only, not for drug, food and household use.