



Current Data Parameters


NAME\_ 0523-47  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters

Date\_ 20240524  
Time 11.59 h  
INSTRUM spect  
PROBHD Z116098\_0490  
PULPROG zgpg  
TD 65536  
SOLVENT DMSO  
NS 16  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.244532 Hz  
AQ 4.0894465 sec  
RG 79.4  
DW 62.450 sec  
DE 6.50 us  
TE 299.4 K  
D1 0.0000000 sec  
TD0 1  
SFO1 400.1524709 MHz  
NUC1 1H  
P1 10.00 usec  
PL1 14.697999 W

F2 - Processing parameters

SI 65536  
SF 400.1500019 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 1.5  
PC 1.5

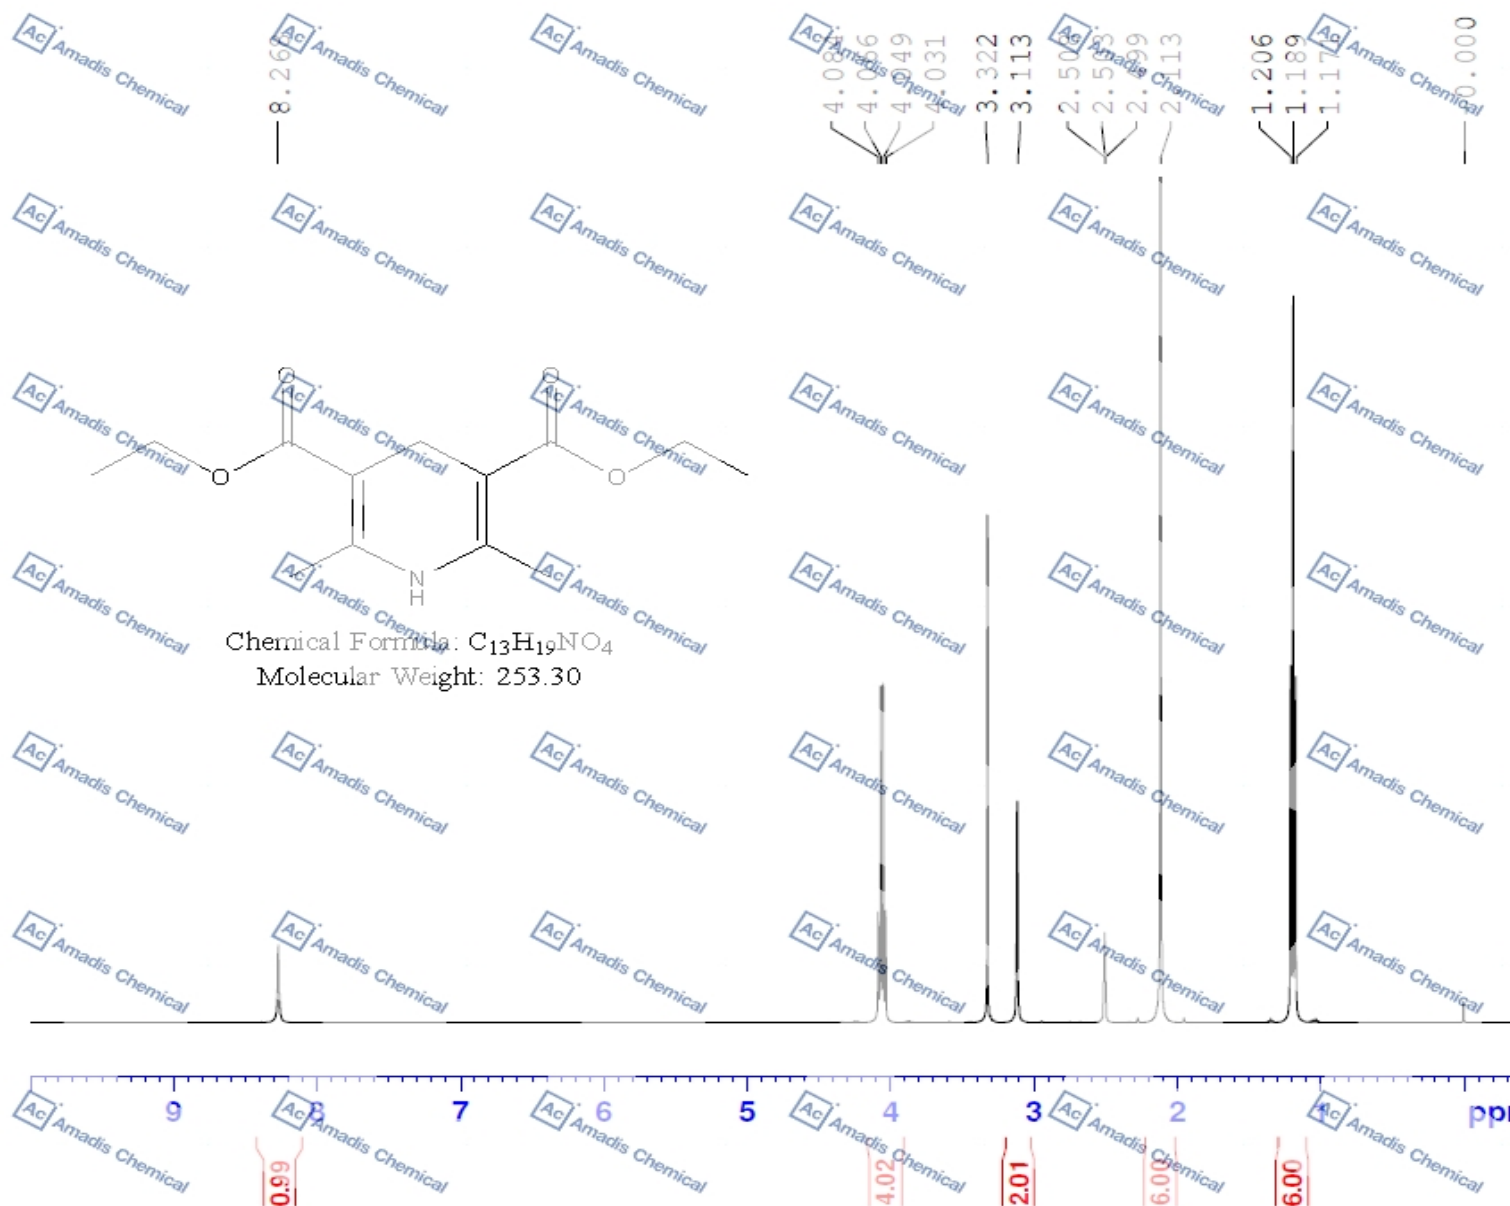

\*For laboratory or manufacturing use only, not for drug, food and household use.