


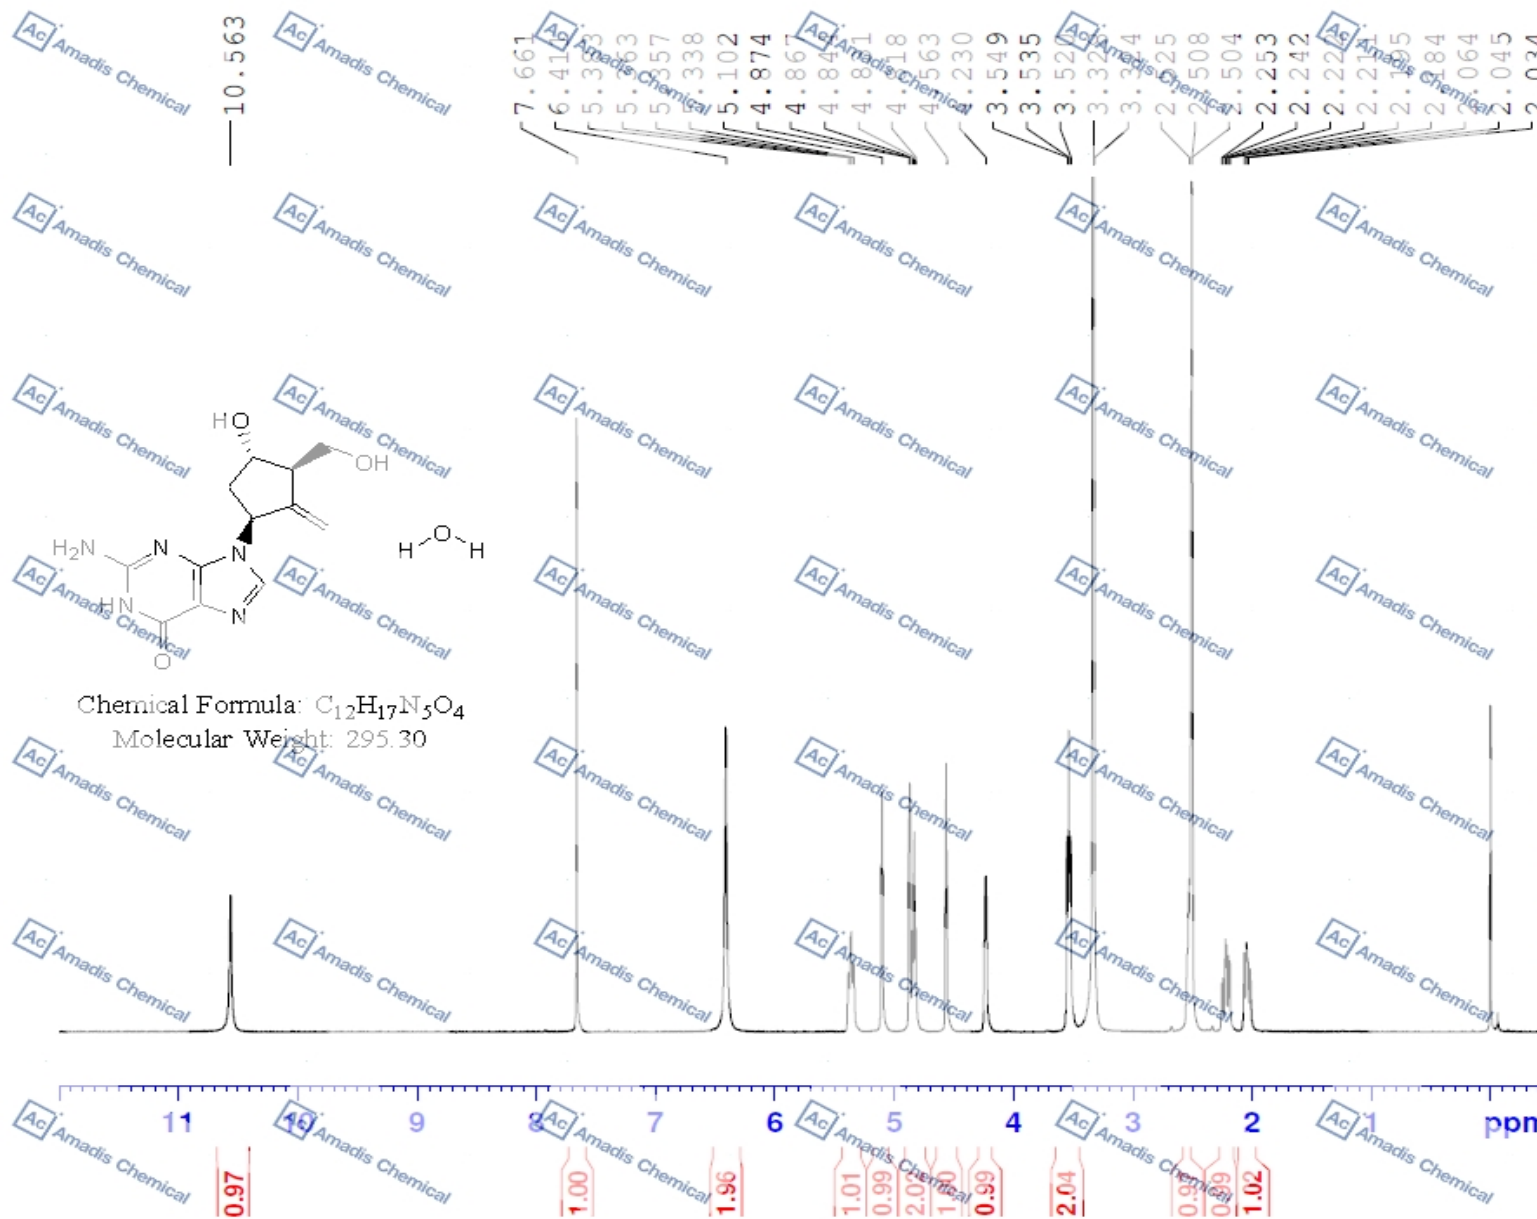

BRUKER

Current Data Parameters

NAME: 0621-48
EXPNO: 10
PROCNO: 1

F2 - Acquisition Parameters

Date_: 20240624
Time: 13.41 h
INSTRUM: spect
PROBHD: Z116098_0490
PULPROG: zgpg
TD: 65536
SOLVENT: DMSO
NS: 16
DS: 2
SWH: 8012.820 Hz
FIDRES: 0.244532 Hz
AQ: 4.0894465 sec
RG: 123.7
DW: 62.400
DE: 6.50 usec
TE: 299.3 K
D1: 1.0000000 sec
TD0: 1
SFO1: 400.1524709 MHz
NUC1: 1H
P1: 10.00 usec
PL1: 14.697999

F2 - Processing parameters

SF: 65536
SF: 400.1500016 MHz
WDW: EM
SSB: 0
LB: 0.30 Hz
GB: 0
PC: 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.