




Current Data Parameters
NAME 1106-5044
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20241107
Time 14.02 h
INSTRUM spect
PROBHD 116098_0490 (1H)
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 512
DWT 62.400 usec
DE 6.50 usec
TE 298.0 K
PC 1.0000000 sec
P1 1.00
P2 1.00
SFO1 400.1524709 MHz
NUC1 1H
P3 1.00 usec
P4 14.6975895 W

F2 - Processing parameters
SI 65536
SF 400.1524709 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

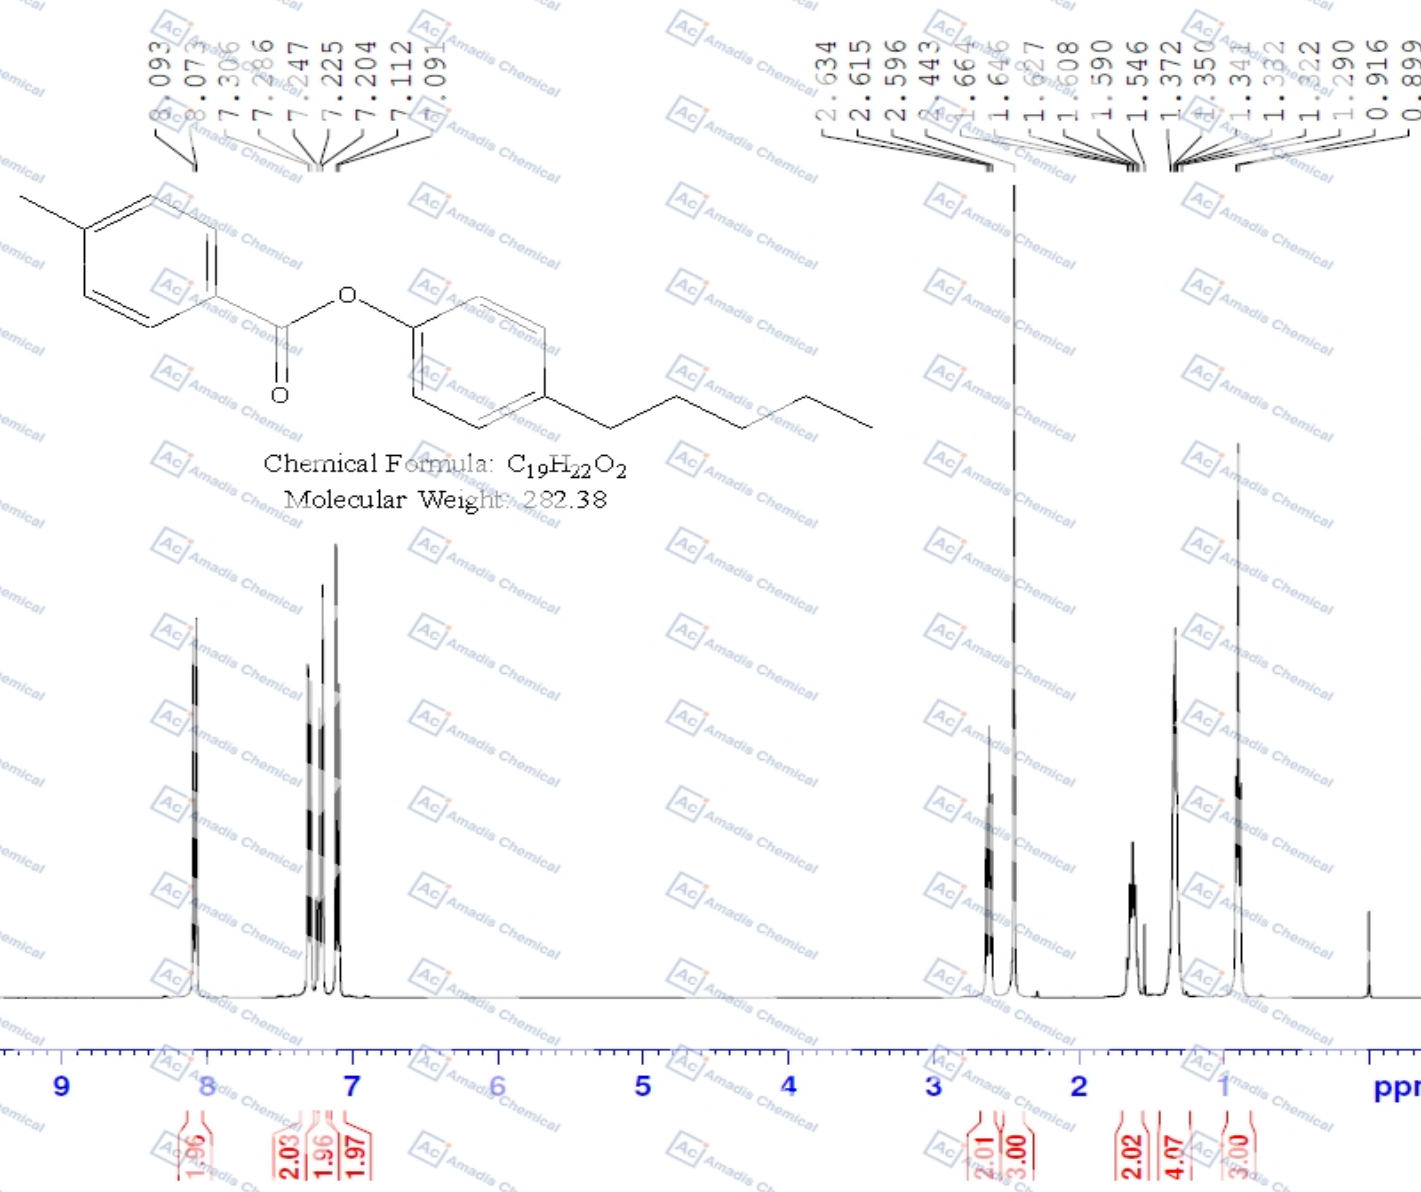

*For R&D use only