


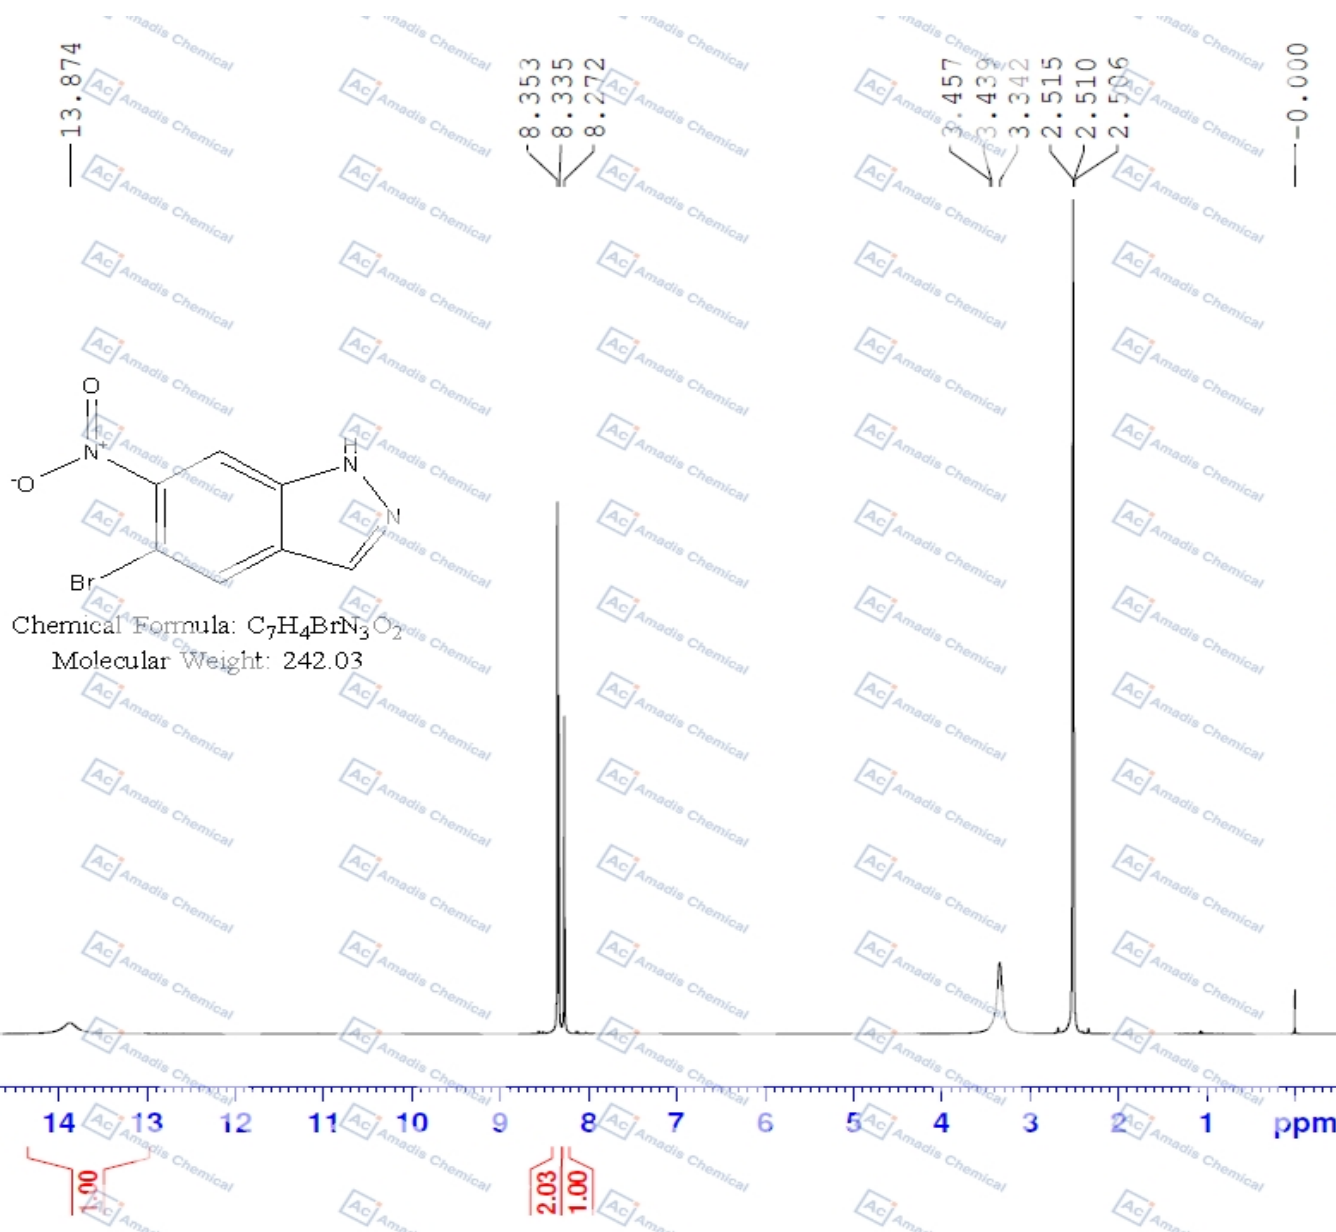

Current Data Parameters
NAME 1101-5030
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters

Date_ 20241104
Time 14.61
INSTRUM spect
PROBHD zgpg30
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.800 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 111.92
DW 62.400 usec
DE 6.50 usec
TE 299.4 K
D1 1.00000000 sec
TD0 4
SFO1 400.1524705 MHz
NUC1 1H
P1 10.00 usec
PLW 14.69799993 W

F2 - Processing parameters

SI 65536
SF 400.1499991 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.