


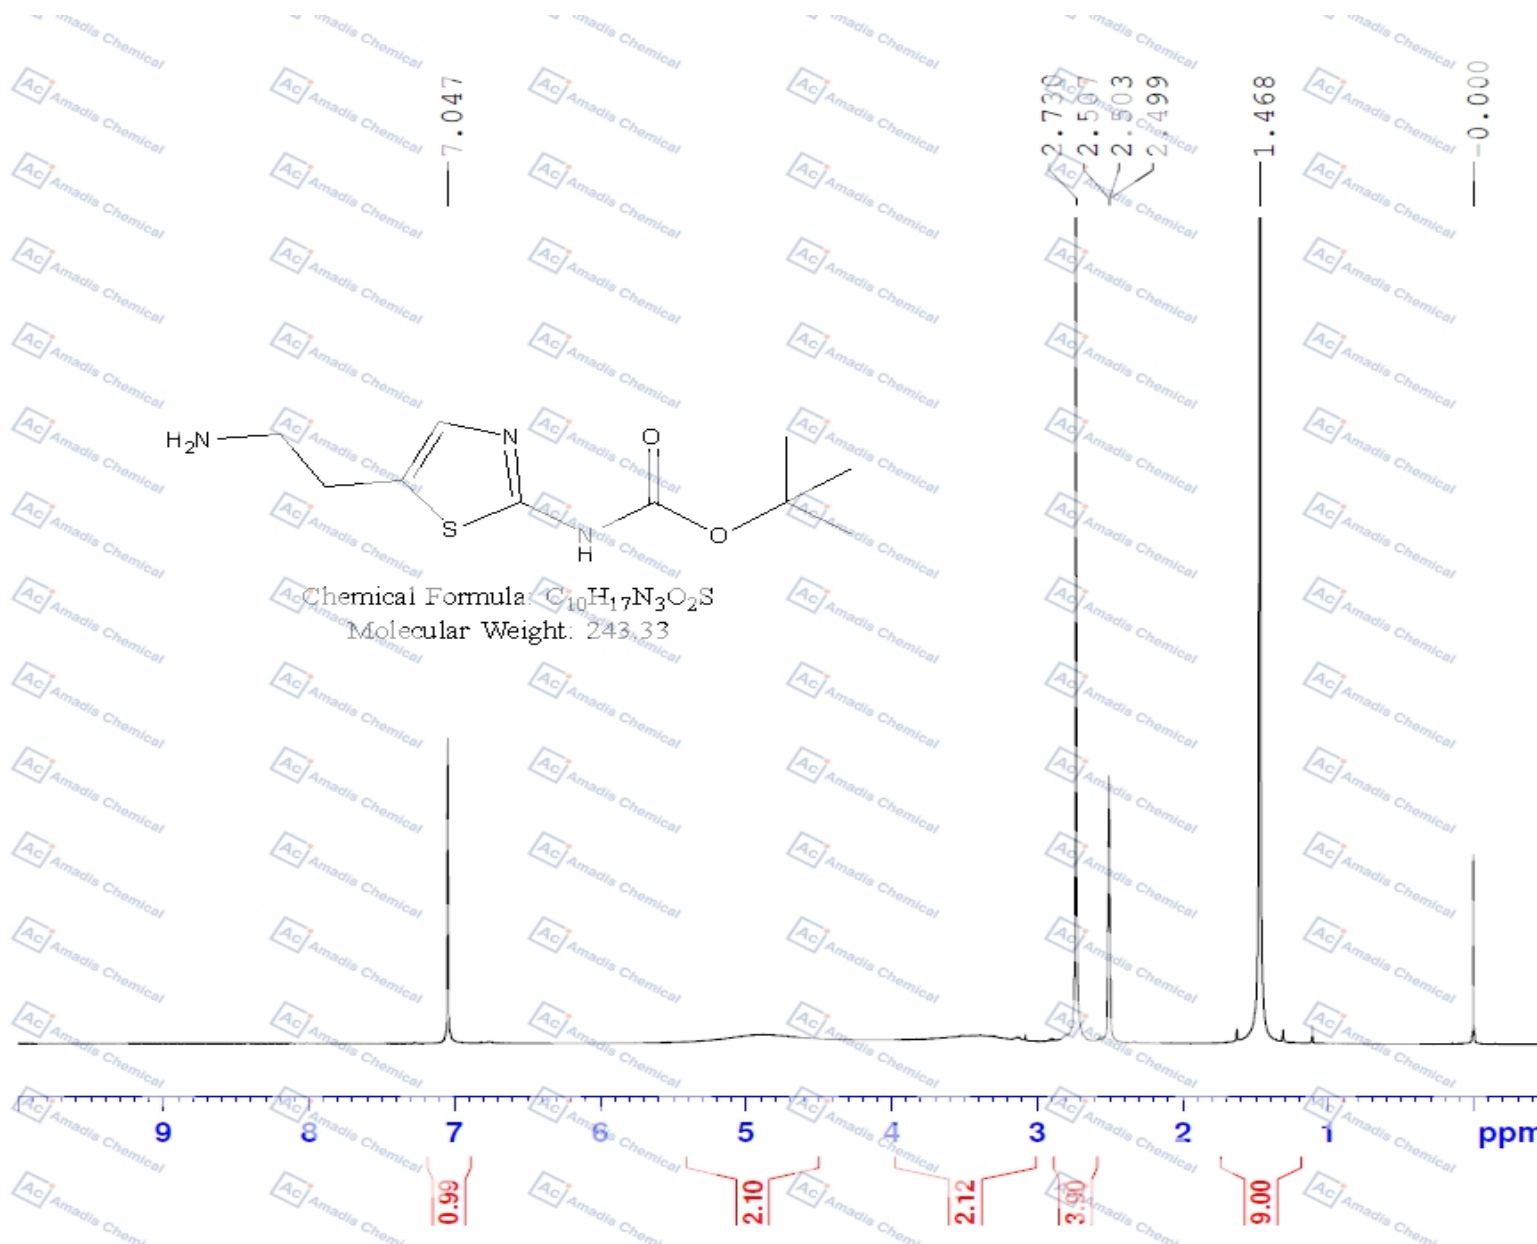

Current Data Parameters

NAME 0902-4957
EXPNO 4
PROCNO 1

F2 - Acquisition Parameters

Date_ 20240903
Time 12.15
INSTRUM spect
PROBHD Z16098_0490 (400 MHz 1H QNP 1H/13C) (1H/13C) (1H/13C)
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 1114.92
DW 62.400 usec
DE 6.50 usec
TE 298.2 K
D1 1.00000000 sec
TDS 4
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 0.00 dB
PL2 14.6979595 W

F2 - Processing parameters

SI 65536
SF 400.1500072 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.