


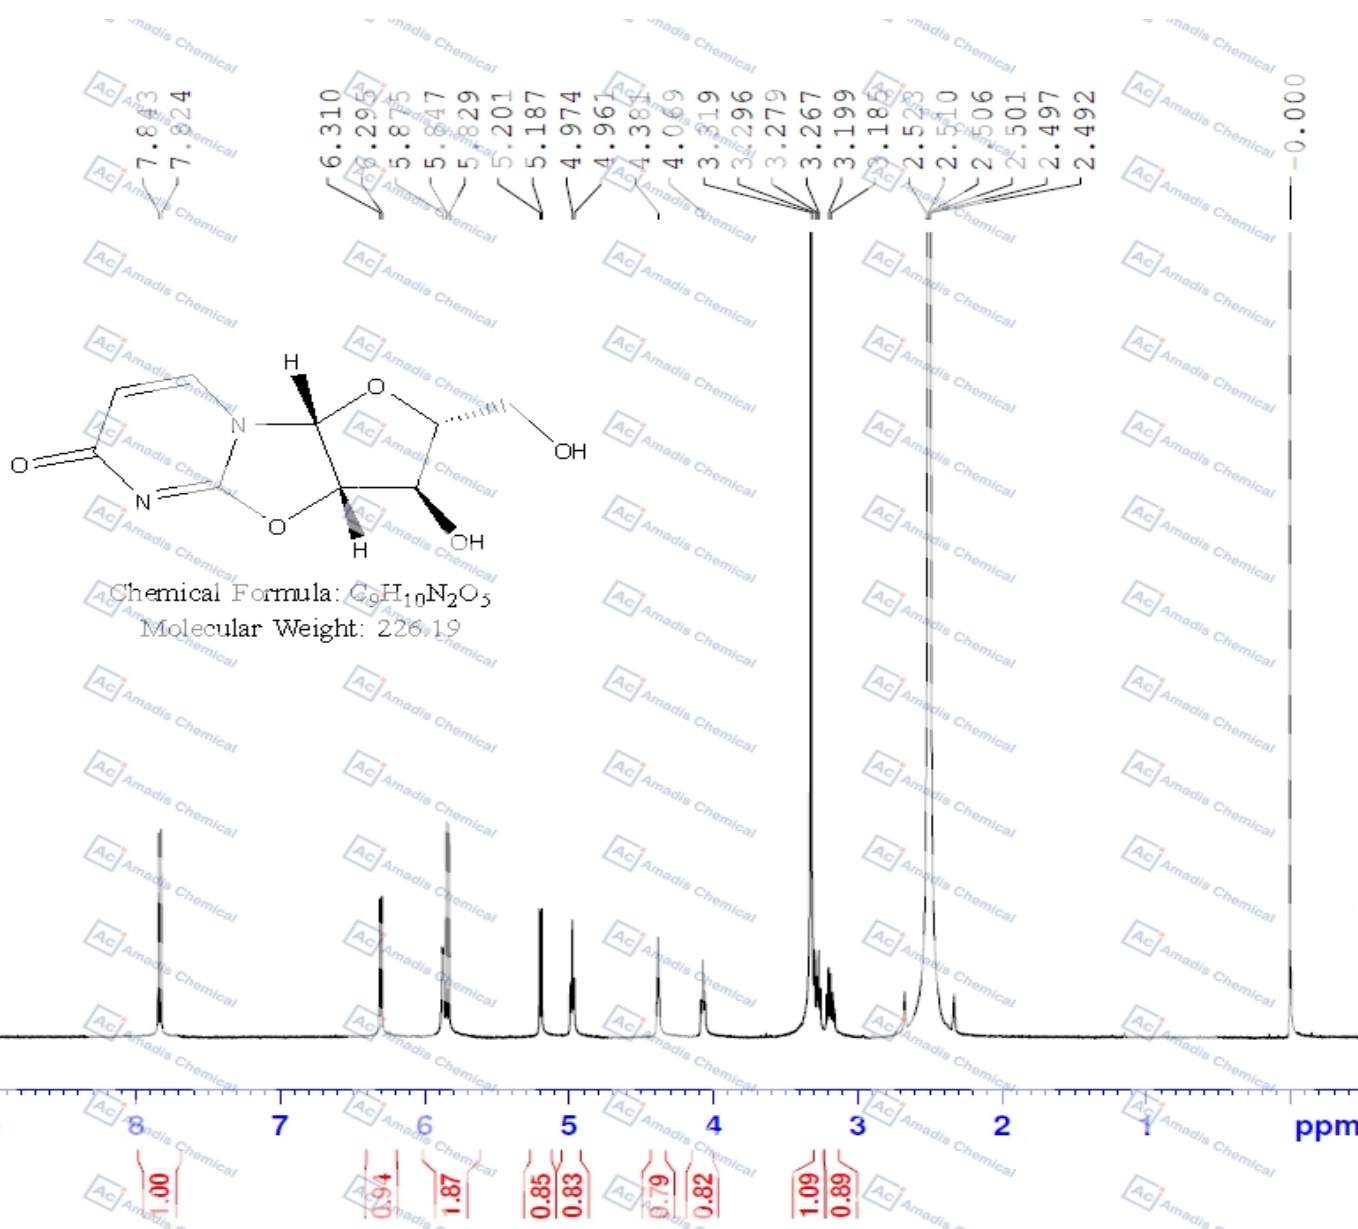

Current Data Parameters
NAME 1031-5029
EXPNO 0
PROCNO 1

F2 - Acquisition Parameters
Date_ 20241101
Time 15:37
INSTRUM spect
PROBHD 5116098_0490 (z)
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 123.07
DN 62.400 usec
DE 6.50 usec
TE 298.3 K
D1 1.00000000 sec
TE0C
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 14.6979993 W

F2 - Processing parameters
SI 65536
SF 400.1500029 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.