



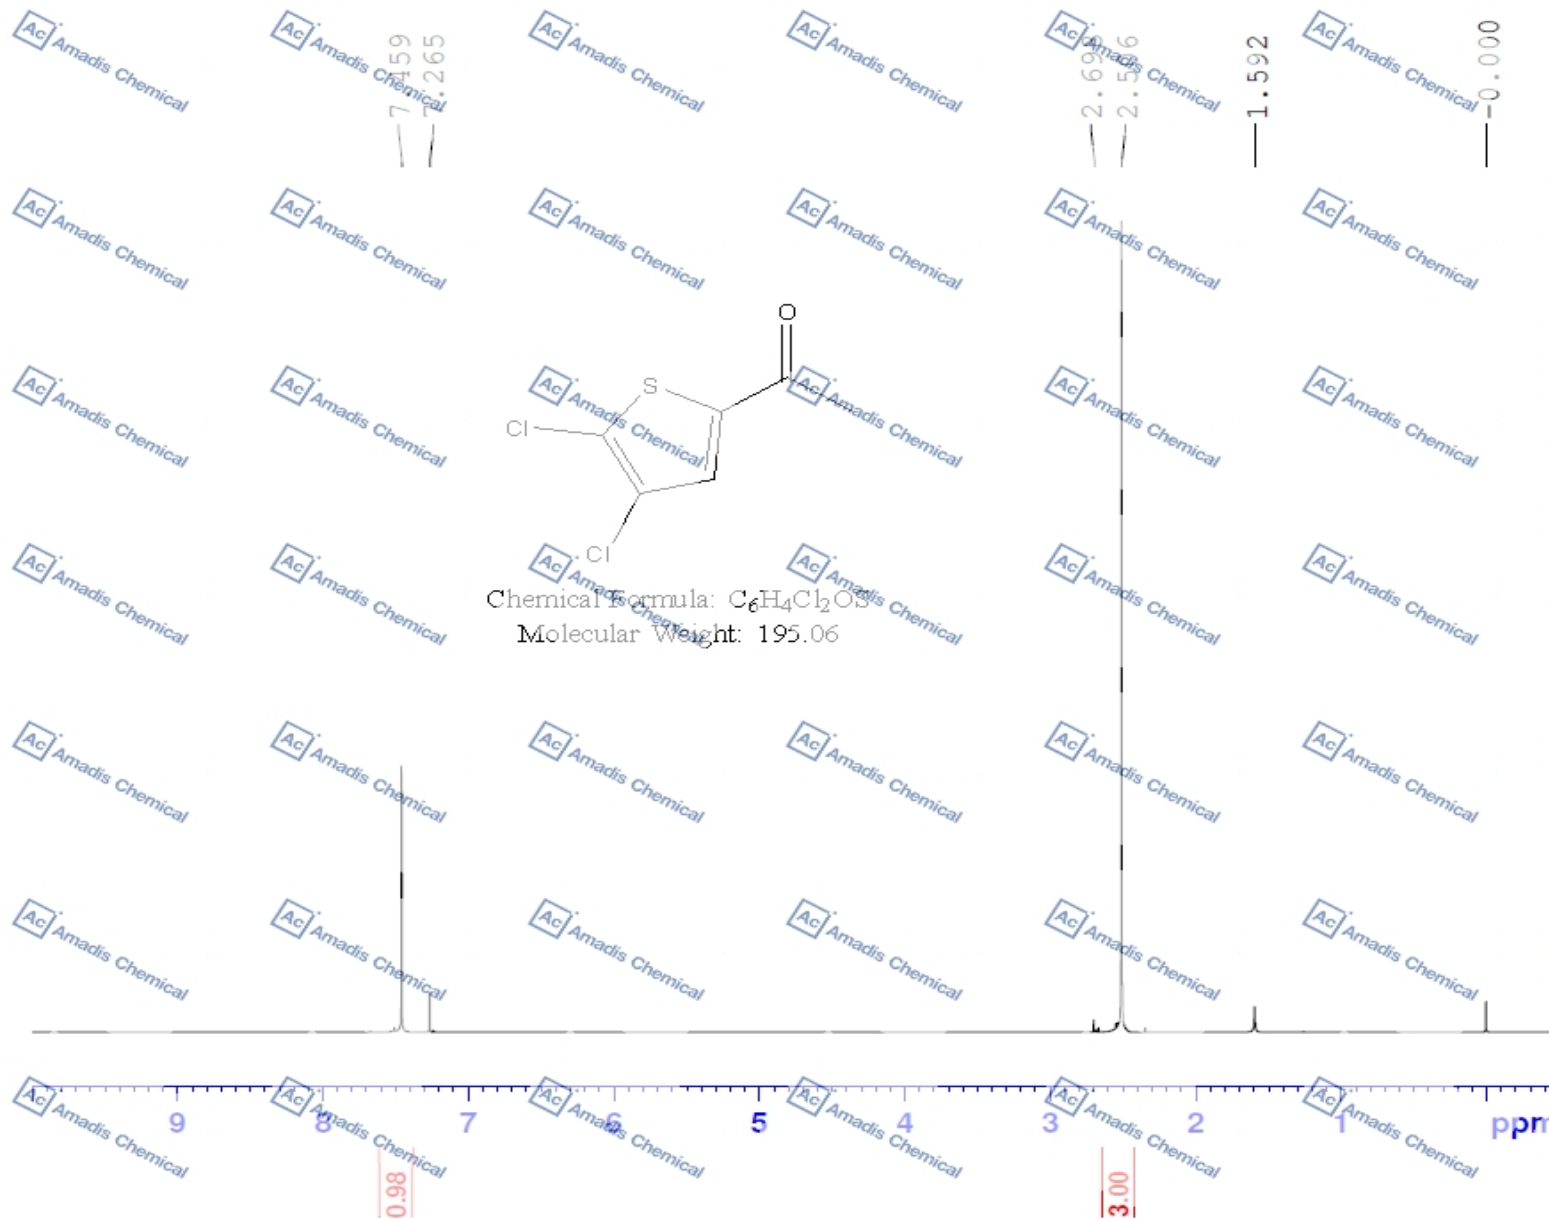

Current Data Parameters
Ac 0517
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240520
Time 12.43 h
INSTRUM spect
PROBHD Z116098_04
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.089465 sec
RG 114.47
DW 62.400 usec
DE 6.50 usec
TE 300.6 K
D1 1.0000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
T1 1.00 usec
PL1 14.6979999 W

F2 - Processing parameters
SI 65536
SF 400.1500078 MHz
WDW EM
SSB 0
LB 30 Hz
GB 0
PC 1.00

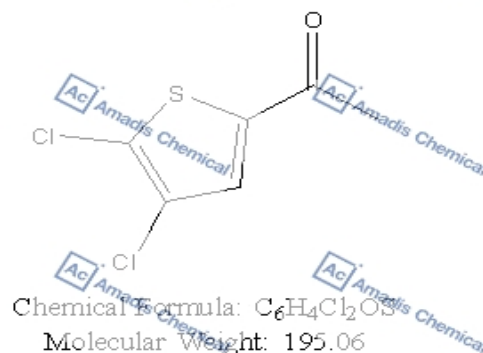

*For laboratory or manufacturing use only, not for drug, food and household use.