


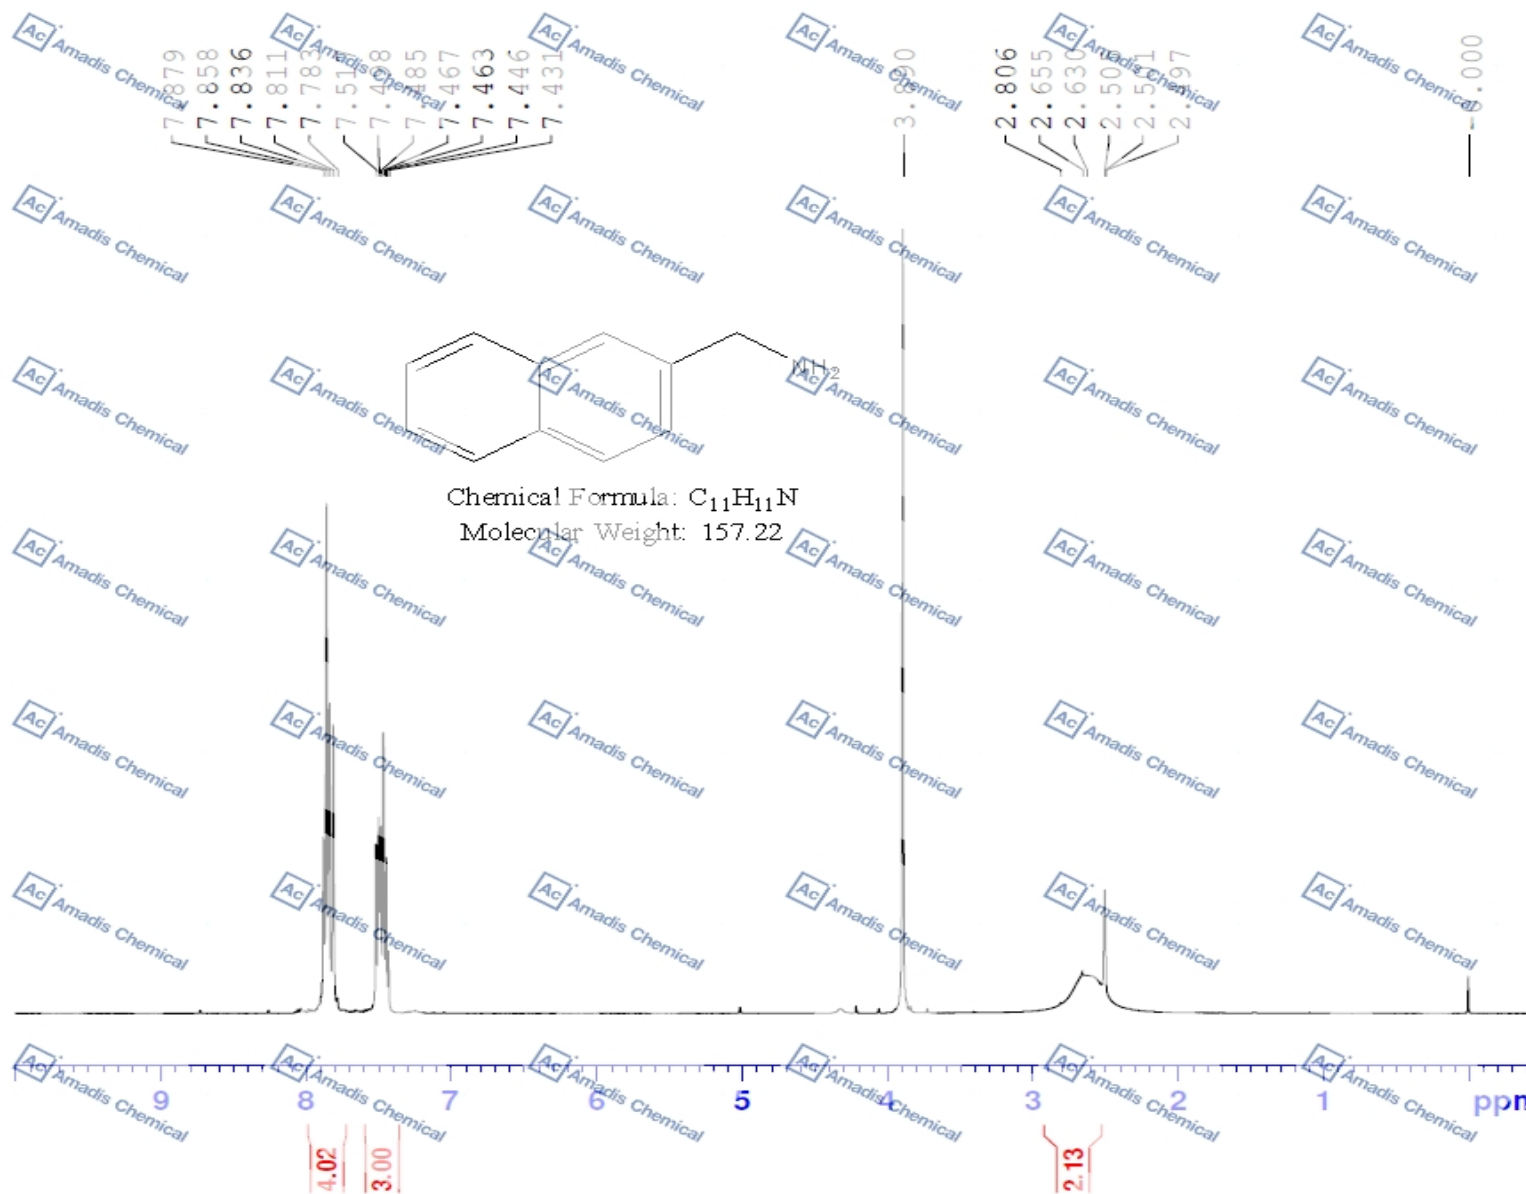

Experiment Data Parameters
NAME: 0614-48
EXPNO: 10
PROCNO: 1

F2 - Acquisition Parameters
Date_: 20240617
Time: 12.47 h
INSTRUM: spect
PULPROG: zgpg30
TD: 65536
SOLVENT: DMSO
NS: 16
DS: 2
SWH: 8012.820 Hz
FIDRES: 0.244532 Hz
AQ: 4.089155 sec
RG: 60.00
DW: 62.400 usec
DE: 6.50 usec
TE: 300.2 K
D1: 1.00000000 sec
TD0: 1
SFO1: 400.1524709 MHz
NUC1: 1H
PC: 16.00 usec
PLW1: 14.69799995

F2 - Processing parameters
SI: 65536
SF: 400.1500027 MHz
WDW: EM
SSB: 0
LB: 0.00 Hz
GB: 0
PC: 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.