


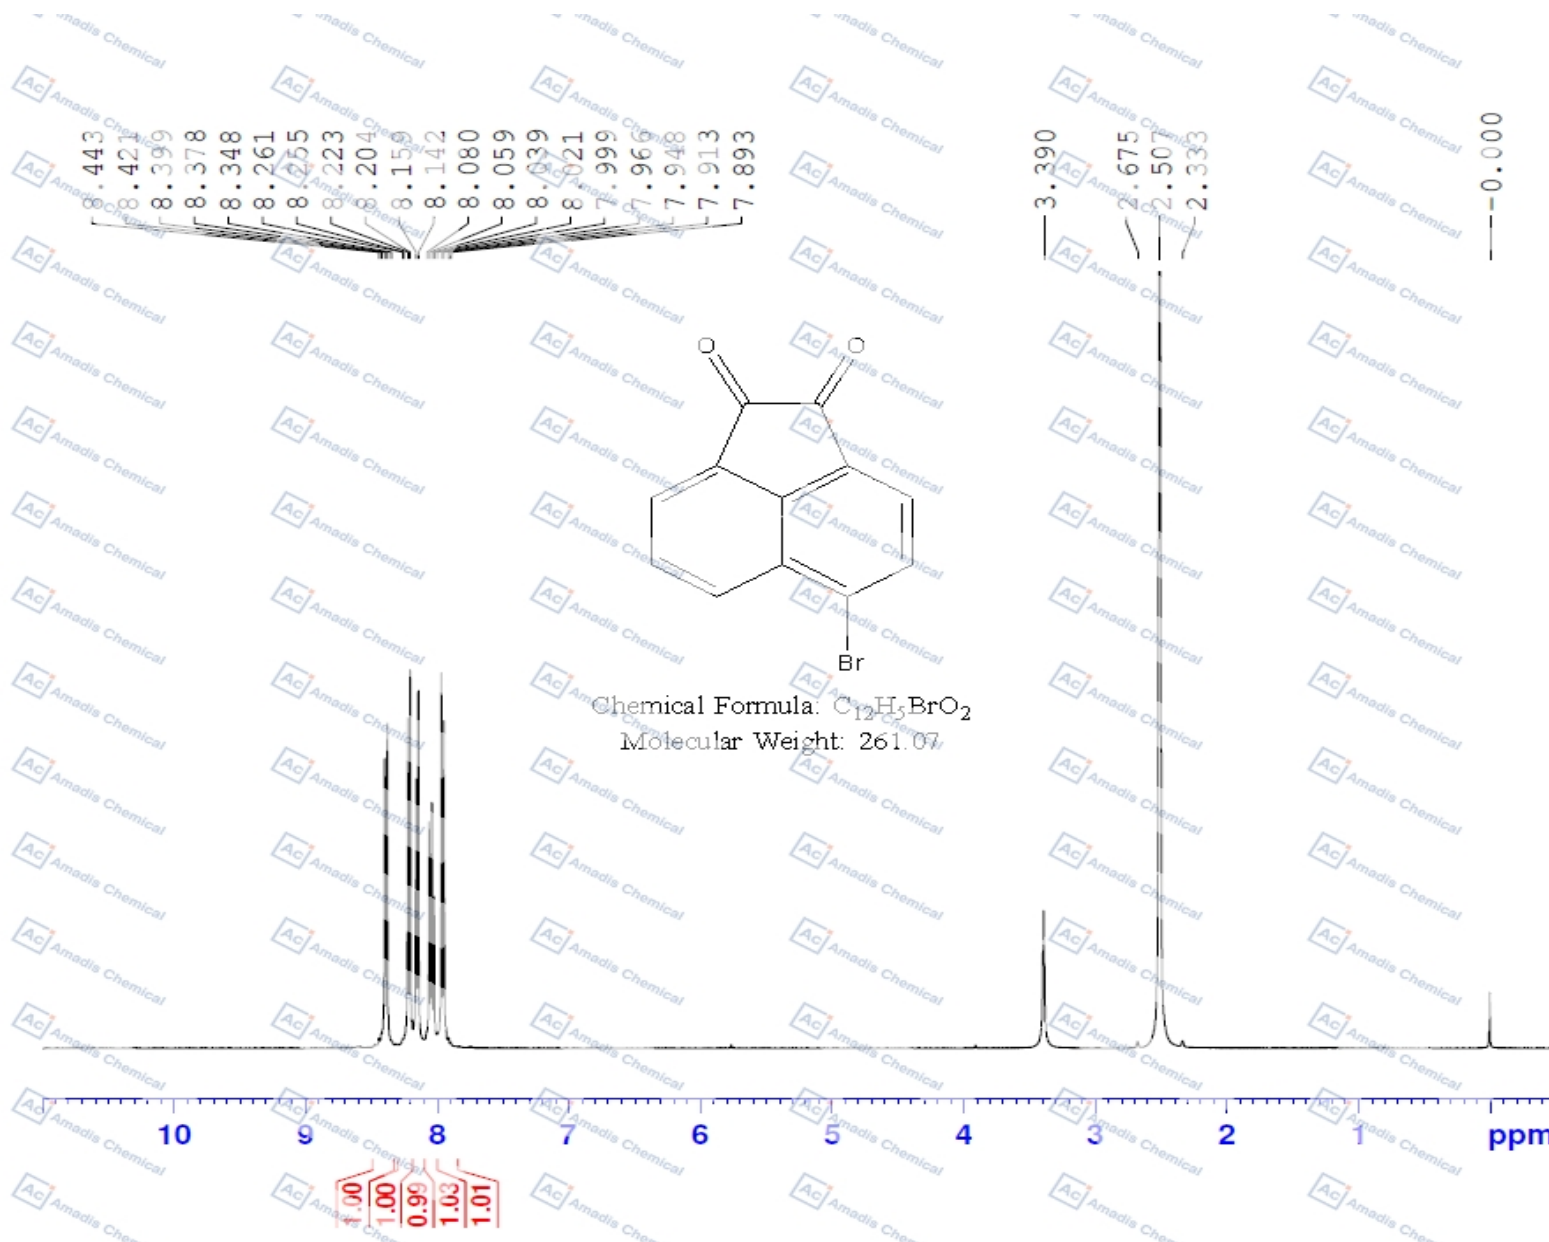

Current Data Parameters
NAME 0224-5160
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250225
Time 15:38:00
INSTRUM spect
PROBHD zgpg098_0490 (4
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 994.69
DW 62.400 usec
DE 6.50 usec
TE 294.8 K
D1 1.00000000 sec
TD0
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 15.59300000 W

F2 - Processing parameters
SI 65536
SF 400.1500003 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.