


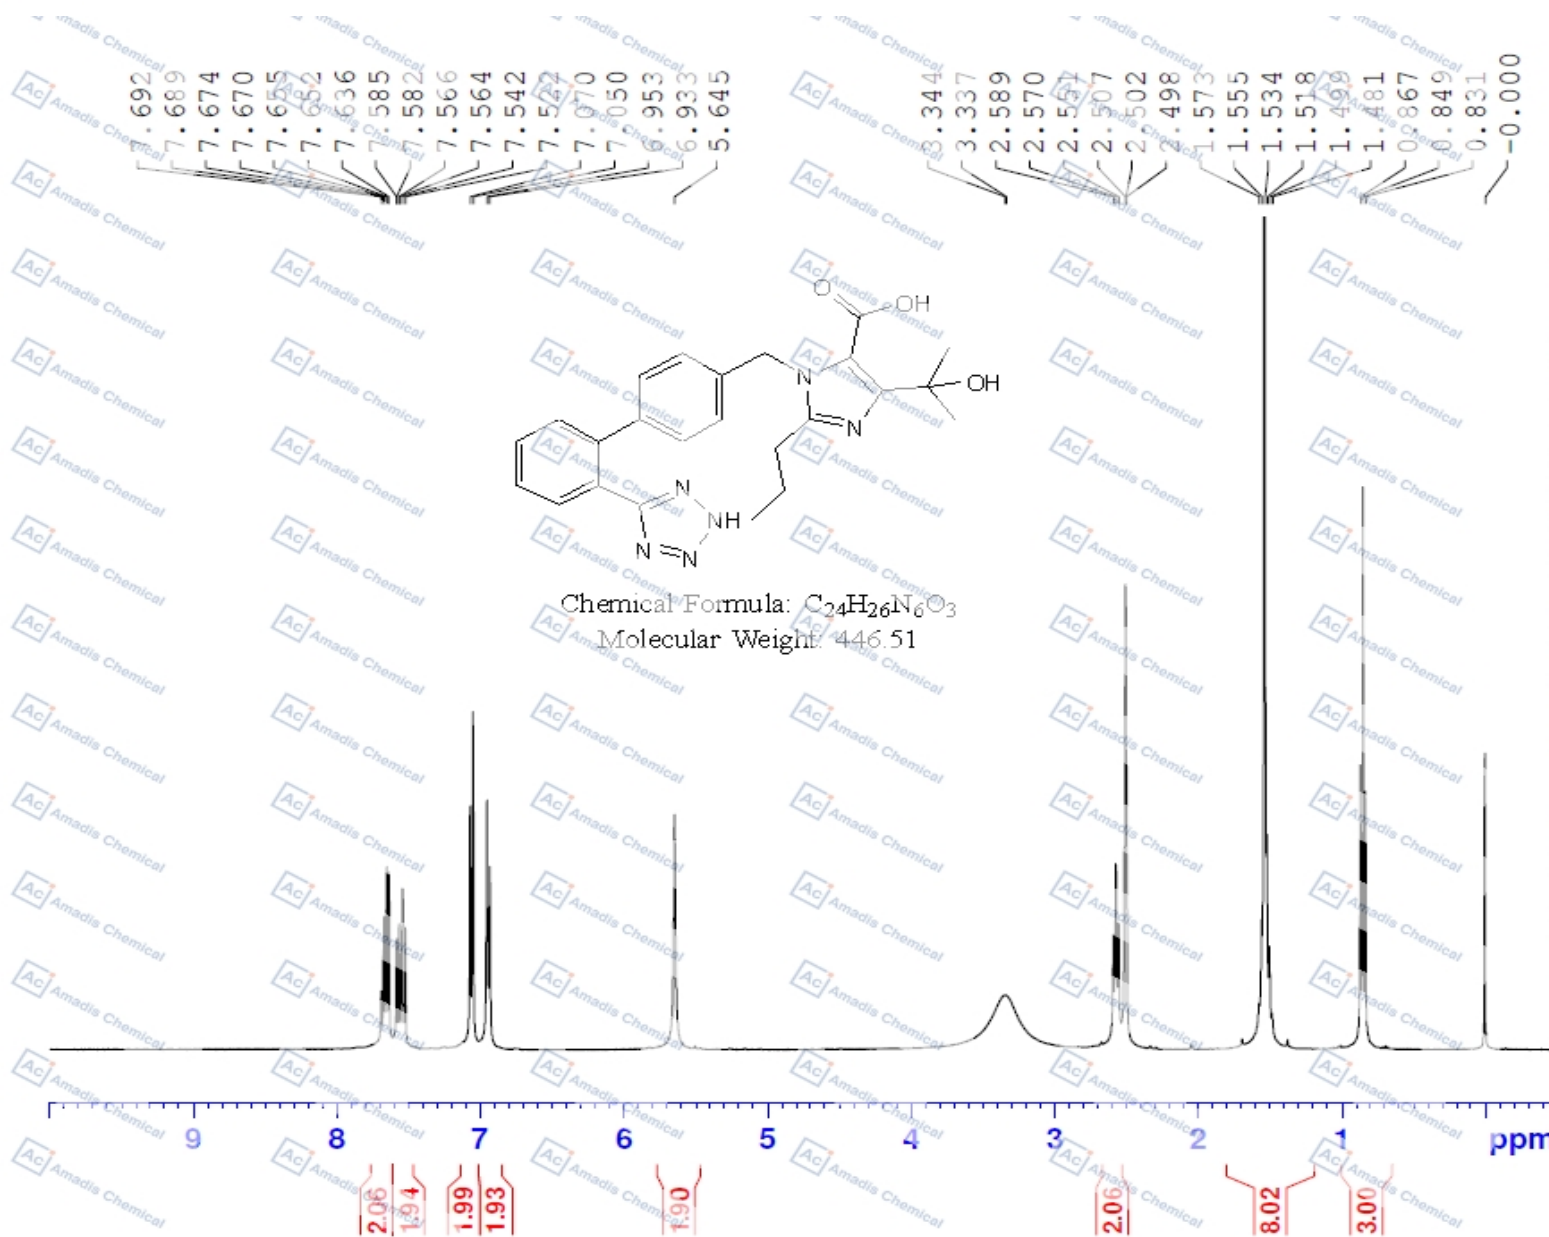

Current Data Parameters
NAME 0826-4947
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240827
Time 12:11 h
INSTRUM spect
PROBHD Z116098_0490
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244392 Hz
AQ 4.0894465 sec
RG 98.69
DW 62.400 usec
DE 6.450 usec
TE 297.8 K
D1 1.00000000 sec
TD0 1
SF 400.1524109 MHz
NUC1 1H
P1 10.00 usec
PIW1 14.69799995 W

F2 Processing parameters
SI 65536
SF 400.1500023 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.