
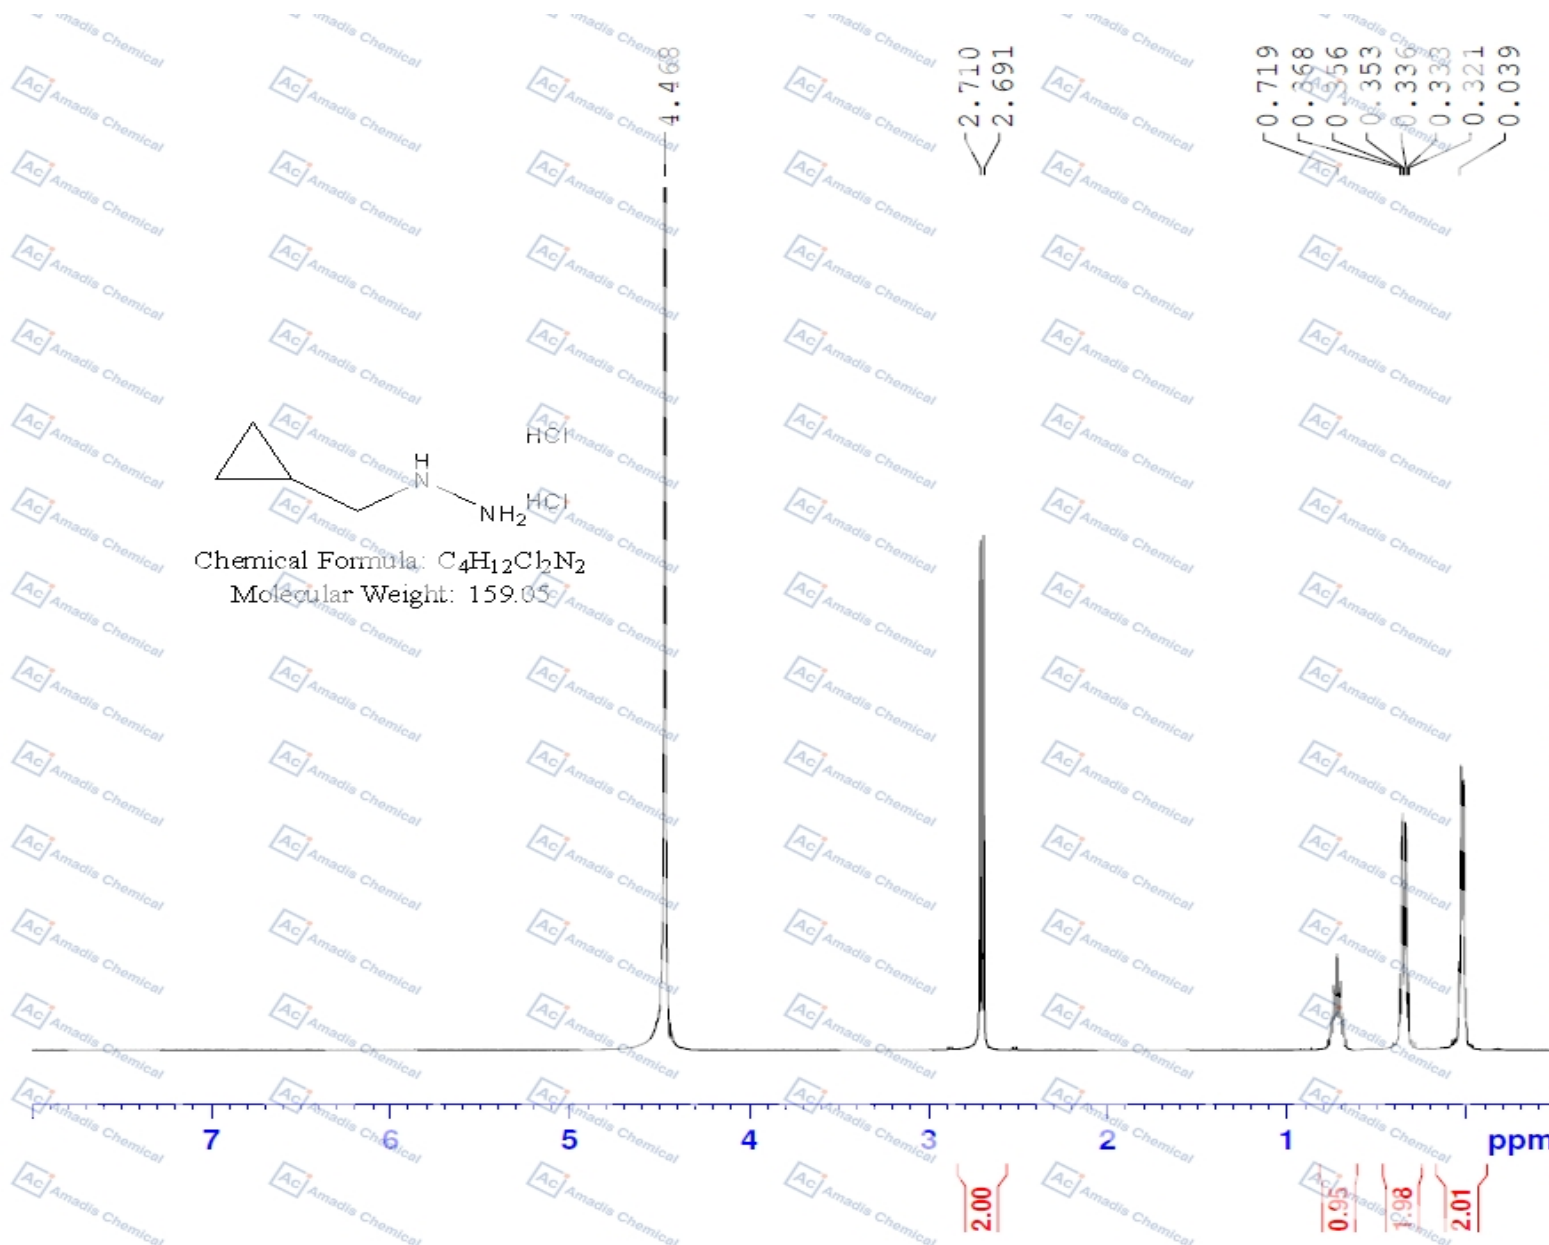


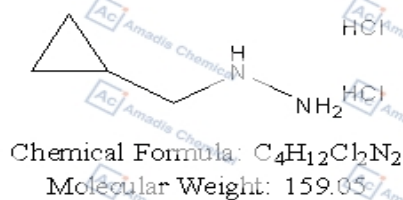

Current Data Parameters

NAME 0623-5339
EXPNO 10
PROCNO 1

Acquisition Parameters

Date_ 20250624
Time 9.47
INSTRUM spect
PROBHD Z116098_0420
PULPROG zgpg30
TD 65536
SOLVENT D2O
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.089465 sec
RG 1113.02
DW 62.400 usec
DE 6.50 usec
TE 298.3 K
D1 1.0000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
PT 10.00 usec
PLW1 15.59300041 W

F2 - Processing parameters

ST 65536
SF 400.1500973 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.