


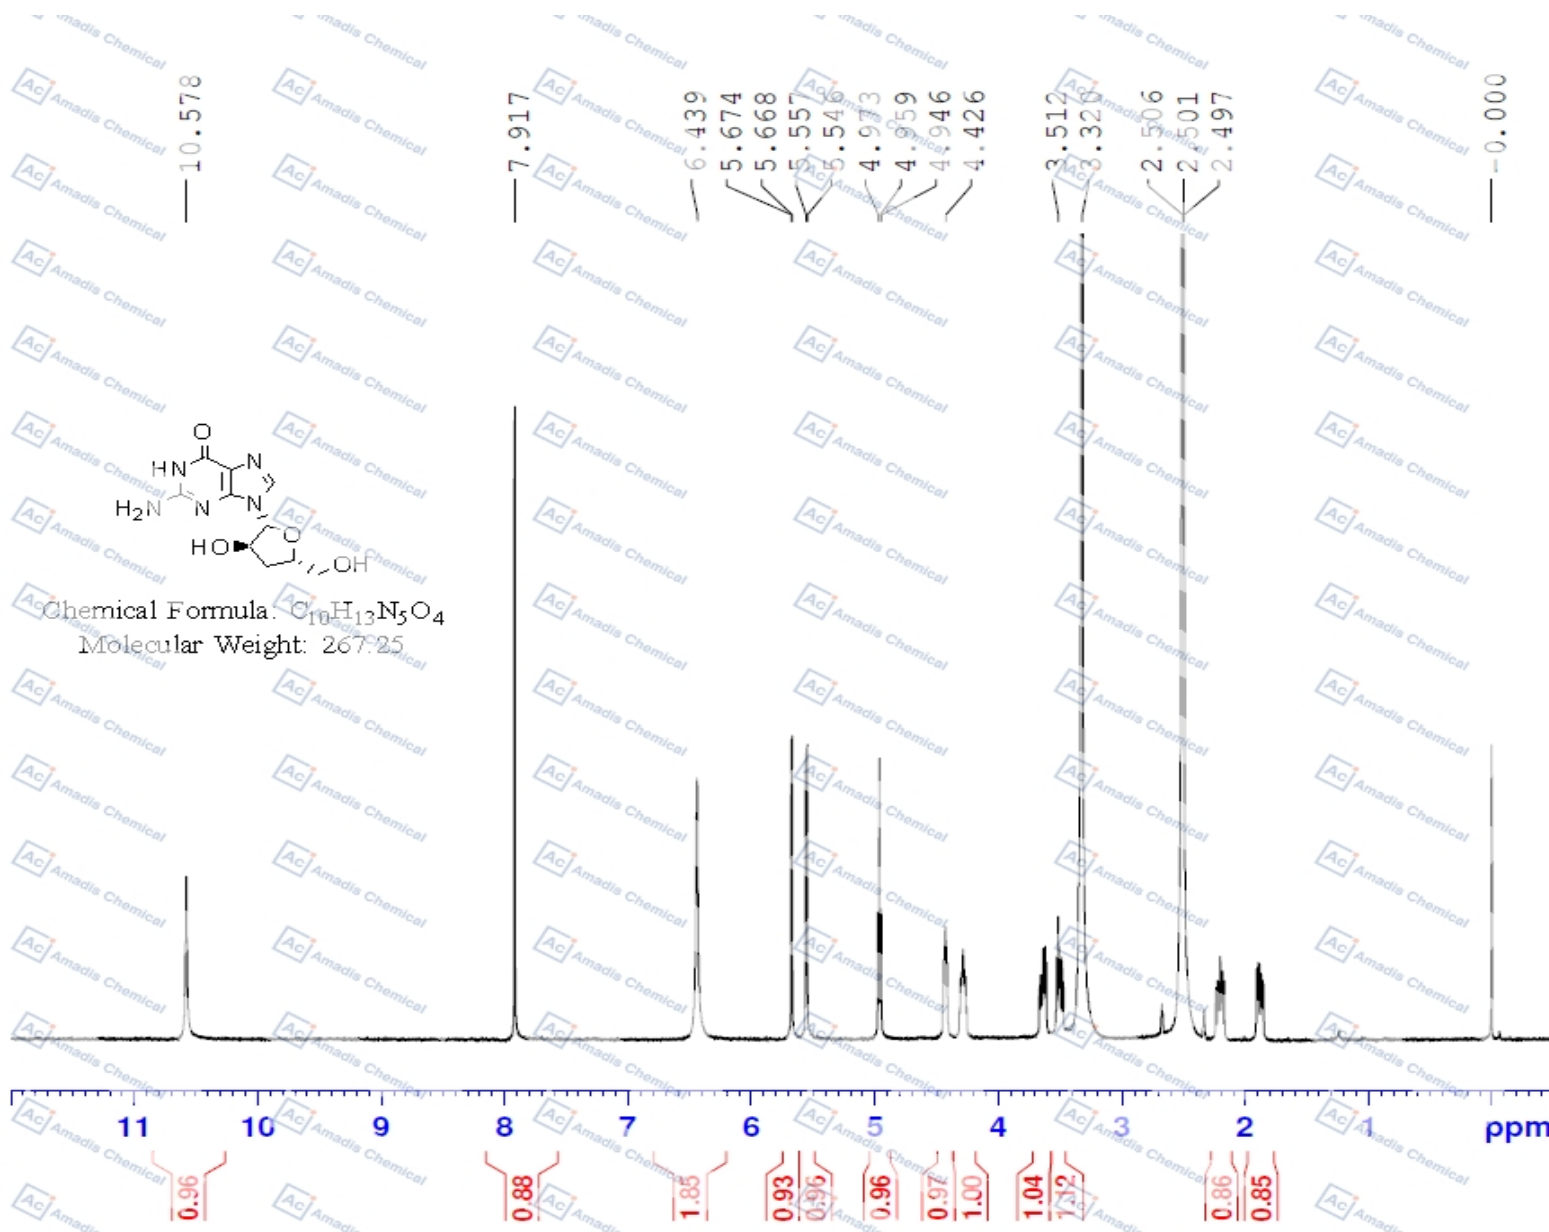

Current Data Parameters
NAME 0506-5274
EXPNO 20
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250507
Time 14:41 h
INSTRUM spect
PROBHD 116098_0490 (4mm) 1H
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 137.37
DW 62.400 usec
DE 6.50 usec
TE 299.1 K
D1 1.0000000 sec
TD0 1
SFO 400.1524789 MHz
NUC1 1H
P1 10.00 usec
PI1 15.59300041 W

F2 - Processing parameters
SI 65536
SF 400.1500025 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.