



Current Data Parameters


NAME 0521-5301
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters

Date_ 20250622
Time 12:49:11
INSTRUM spect
PROBHD zgpg3000-0490 (16098)
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 79.19
DW 62.500 usec
DE 6.50 usec
TE 299.0 K
D1 1.0000000 sec
TDO
SFO1 400.1524709 MHz
NUC1 1H
PT 10.00 usec
PL1 0.00
PL2 15.59306544 W

F2 - Processing parameters

SI 65536
SF 400.1508922 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
CB 0
PC 1.00

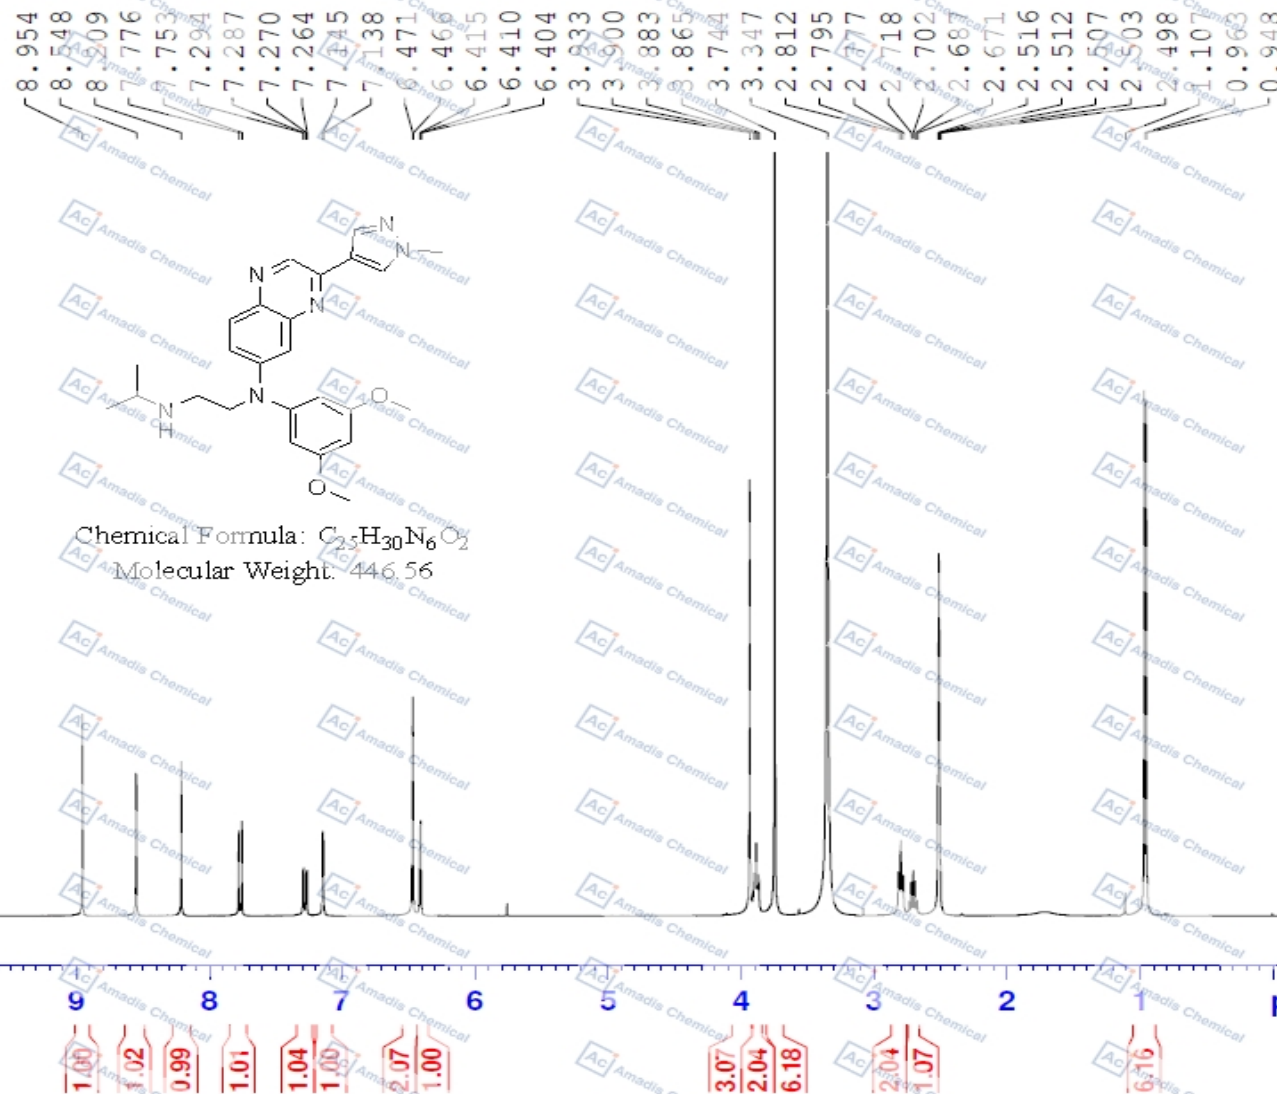

*For laboratory or manufacturing use only, not for drug, food and household use.