





Current Data Parameters
NAME 0423-5260
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters

Date 20250424
Time 11:04 h
INSTRUM spect
PROBHD 116098_0490 (zg30)
PULPROG 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244531 Hz
AQ 4.0894465 sec
RG 98.69
DW 62.400 usec
DE 6.50 usec
TE 298.5 K
D1 1.0000000 sec
TD 65536
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PIPA 15.5930004 W

F2 - Processing parameters

SI 65536
SF 400.1500001 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

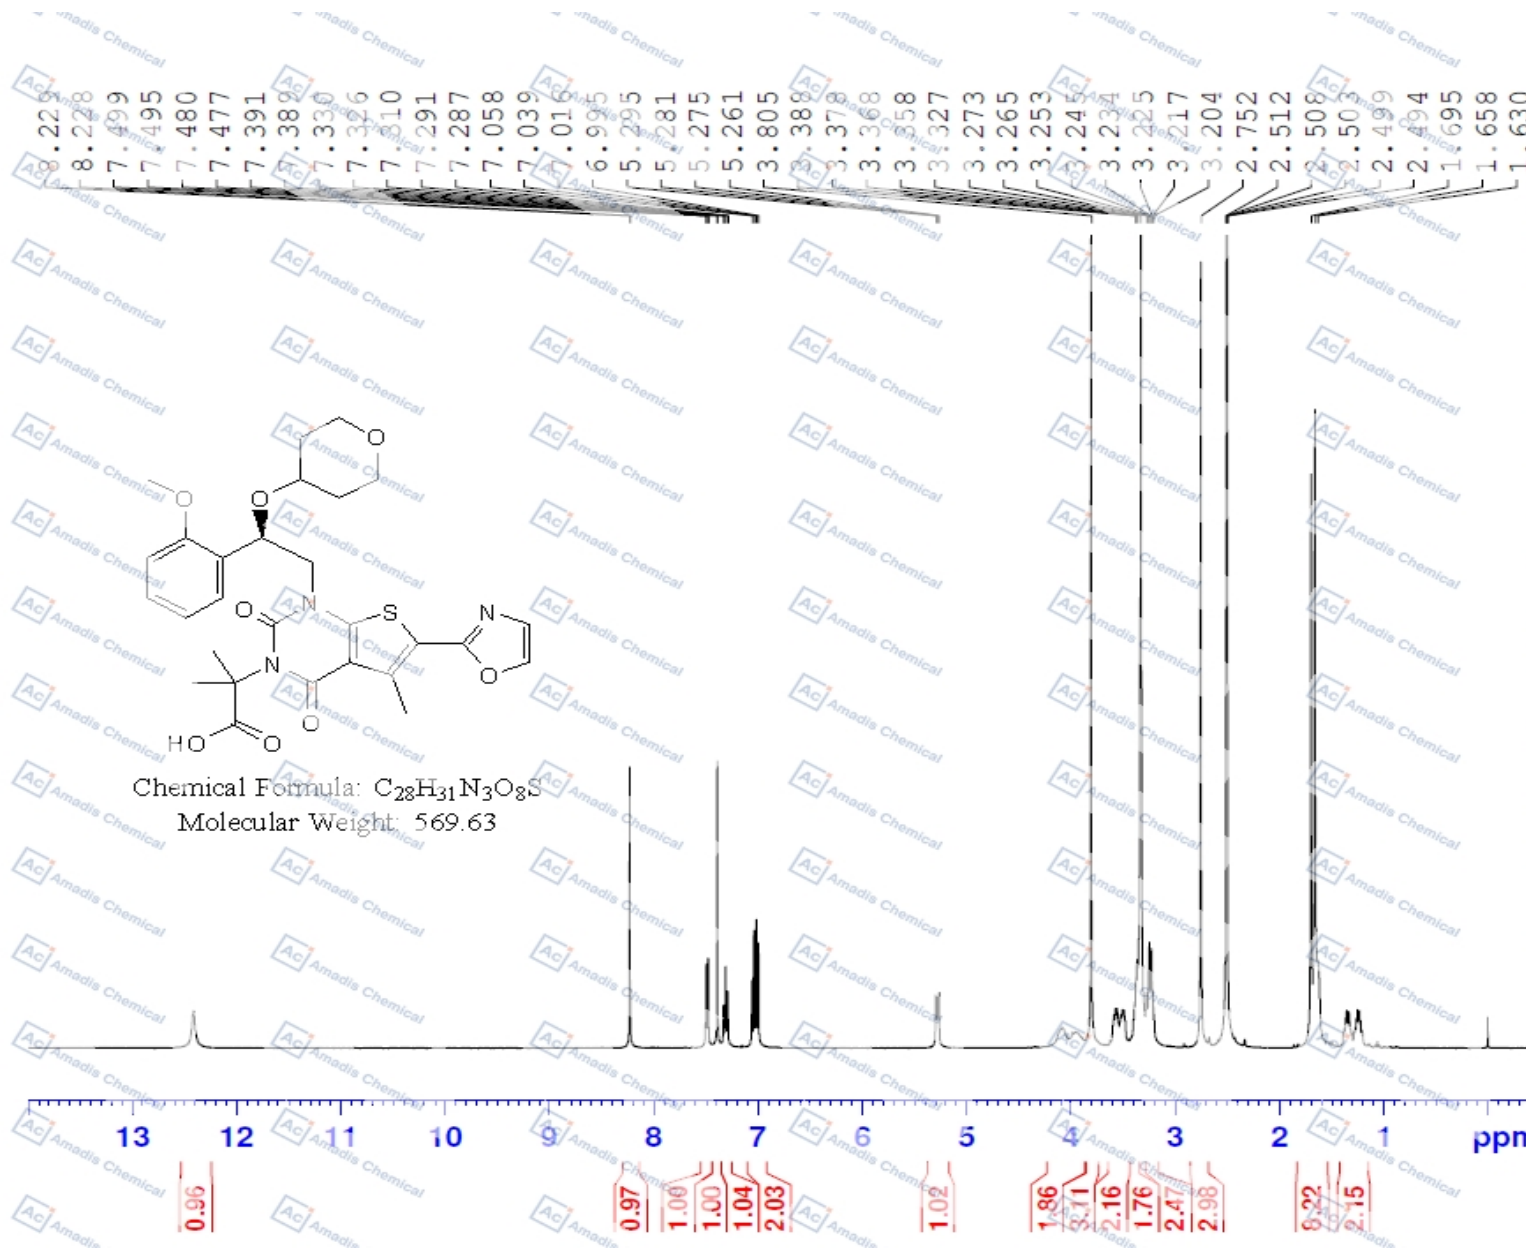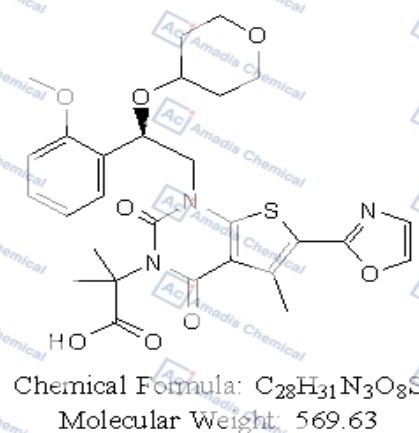

*For laboratory or manufacturing use only, not for drug, food and household use.