


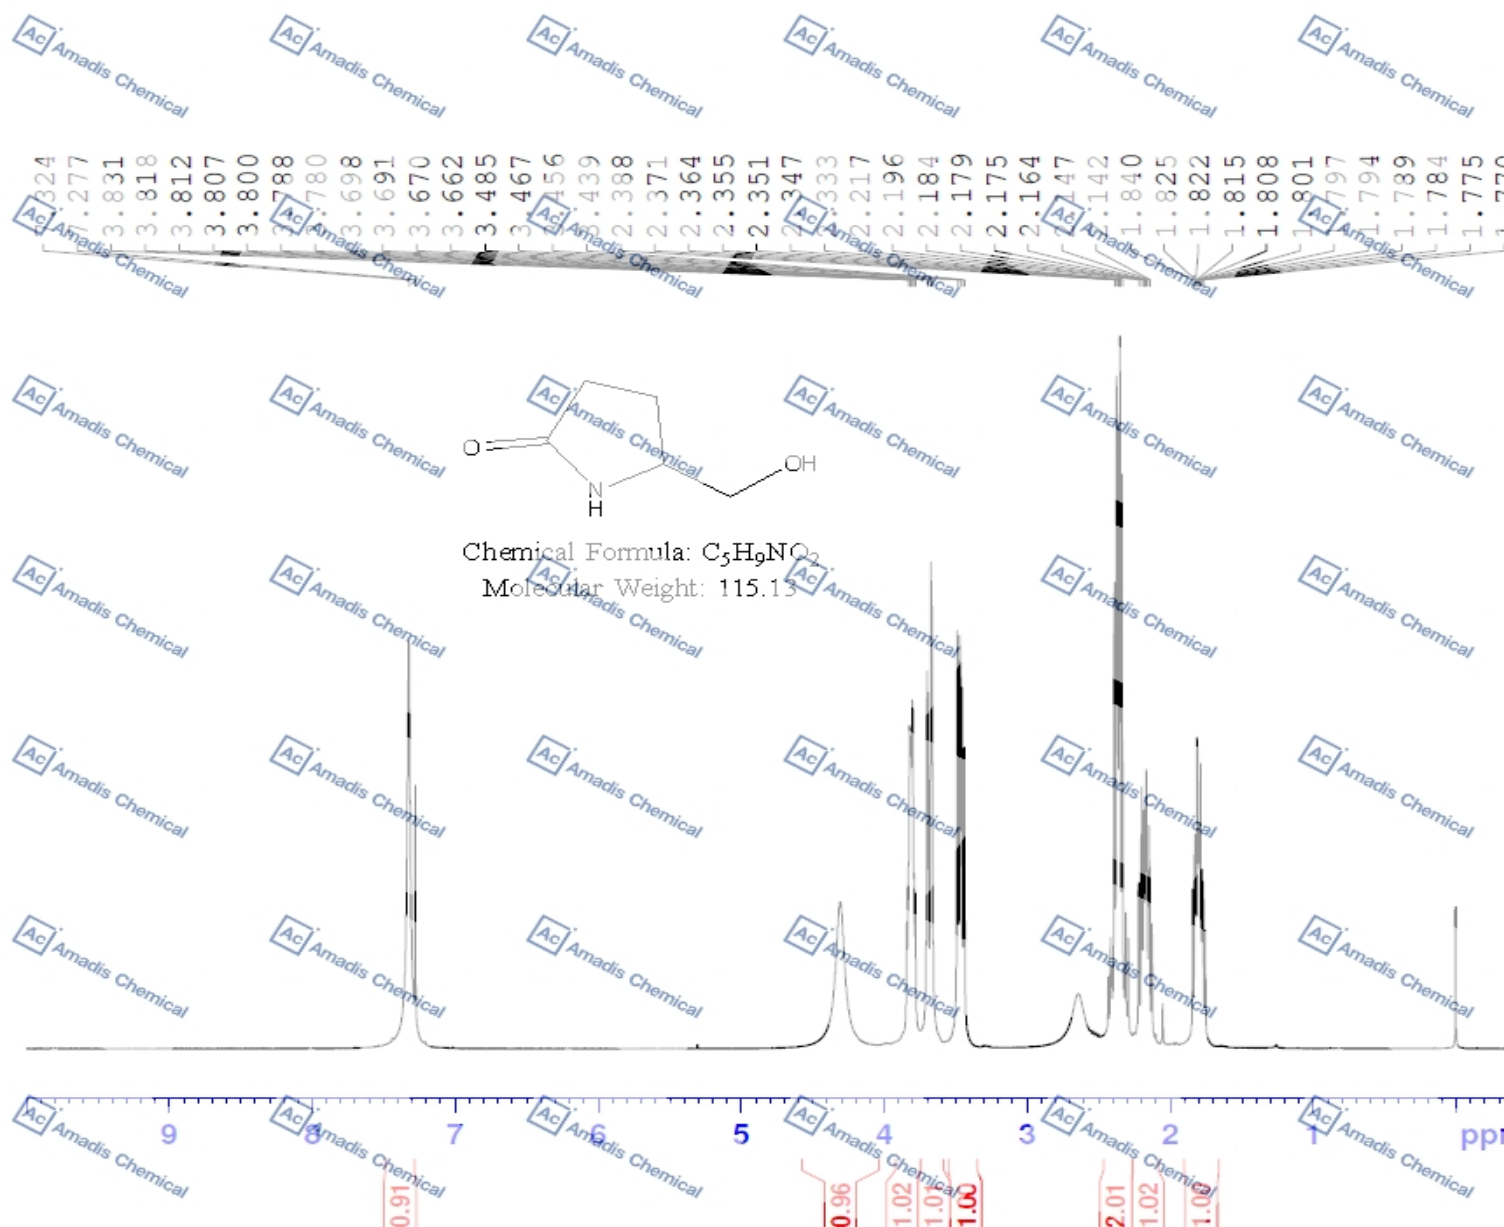

Current Data Parameters
NAME 0613-48
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240614
Time 12.06 h
INSTRUM spect
PRF 7116098.0490
PULPROG zgpg
TD 65536
SOLVENT CDC13
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.08944 sec
RG 67
DW 62.400 usec
DE 6.50 usec
TE 298.4 K
D1 1.00000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10 usec
PLW1 14.69799999

F2 - Processing parameters
SI 65536
SF 400.1500028 MHz
WDW EM
SSB 0
LB 0.0 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.