



Current Data Parameters



NAME 0207-5138
EXPNO 16
PROCNO 1

F2 Acquisition Parameters

Date_ 20250208
Time 10.34
INSTRUM spect
PROBHD z16098_0490
PULPROG zgpg30
TD 65536
SOLVENT D2O
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 111.92
DW 62.400 usec
DE 6.50 usec
TE 297.3 K
D1 1.00000000 sec
TD0
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 15.59300041 W

F2 - Processing parameters

SI 65536
SF 400.1500000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

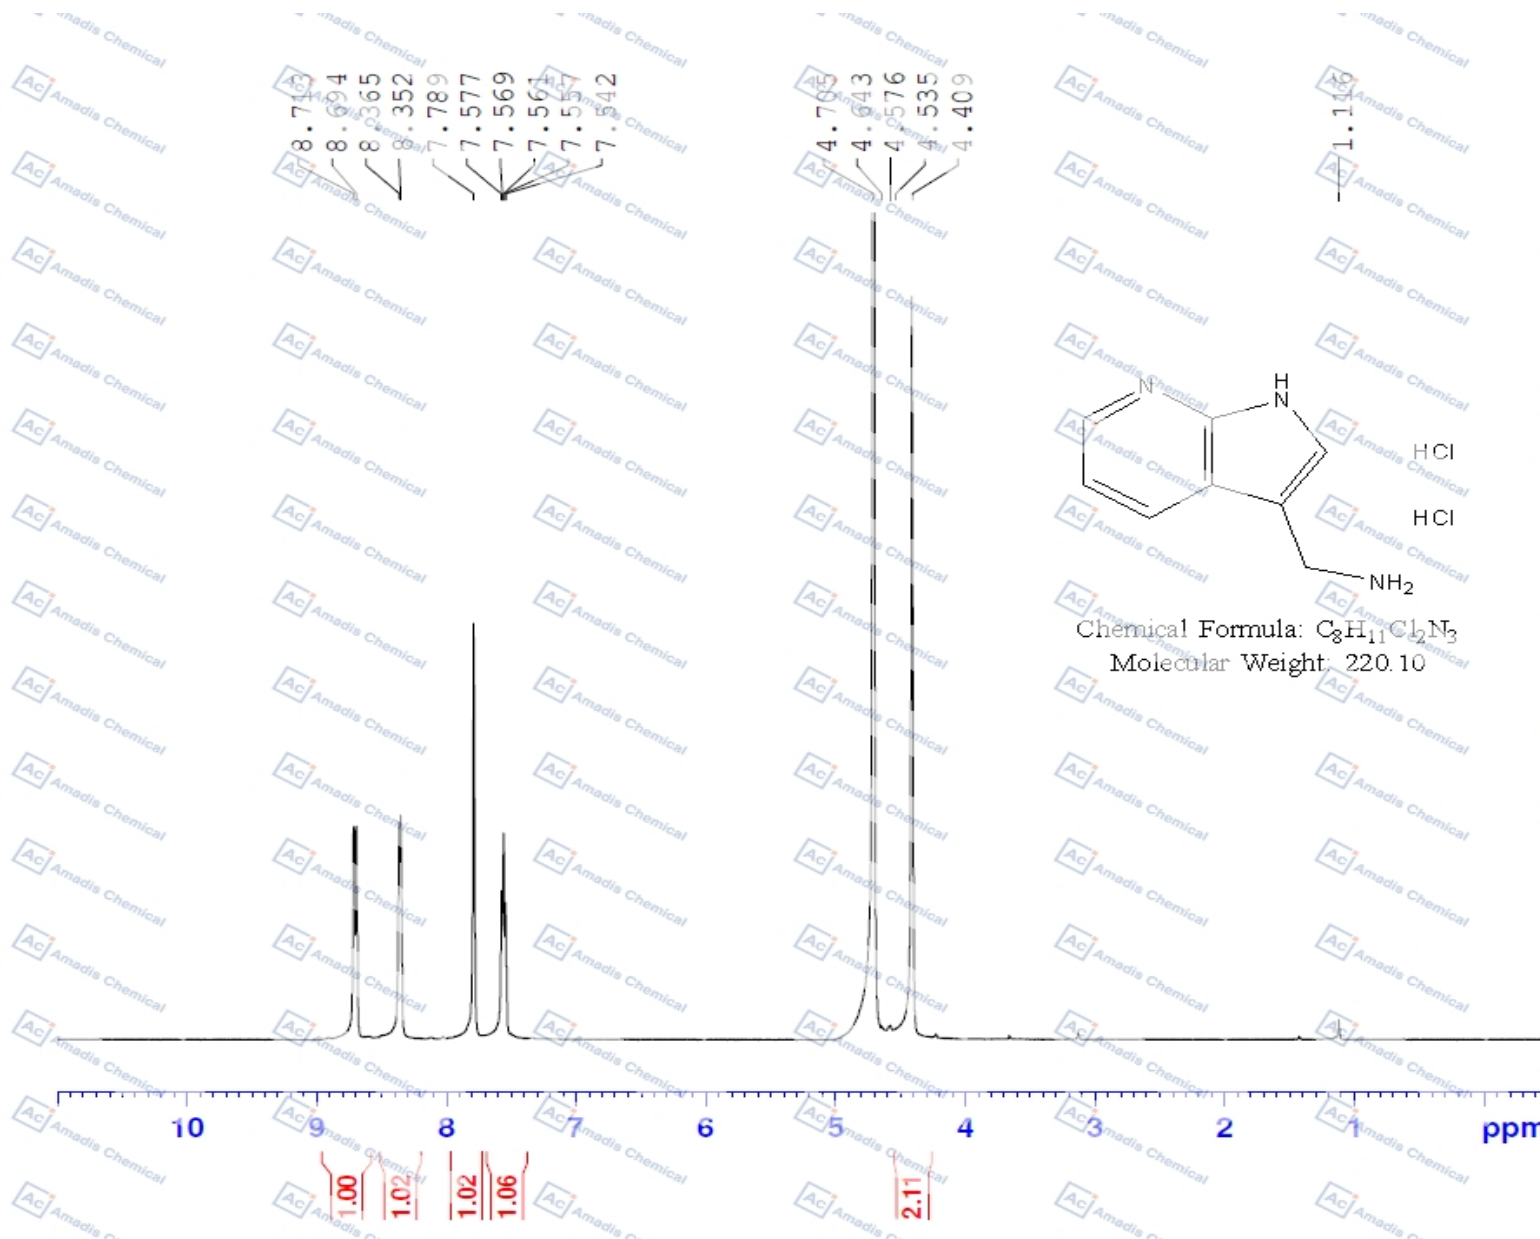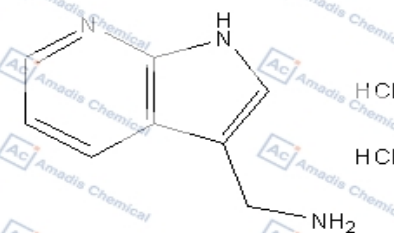

*For laboratory or manufacturing use only, not for drug, food and household use.