


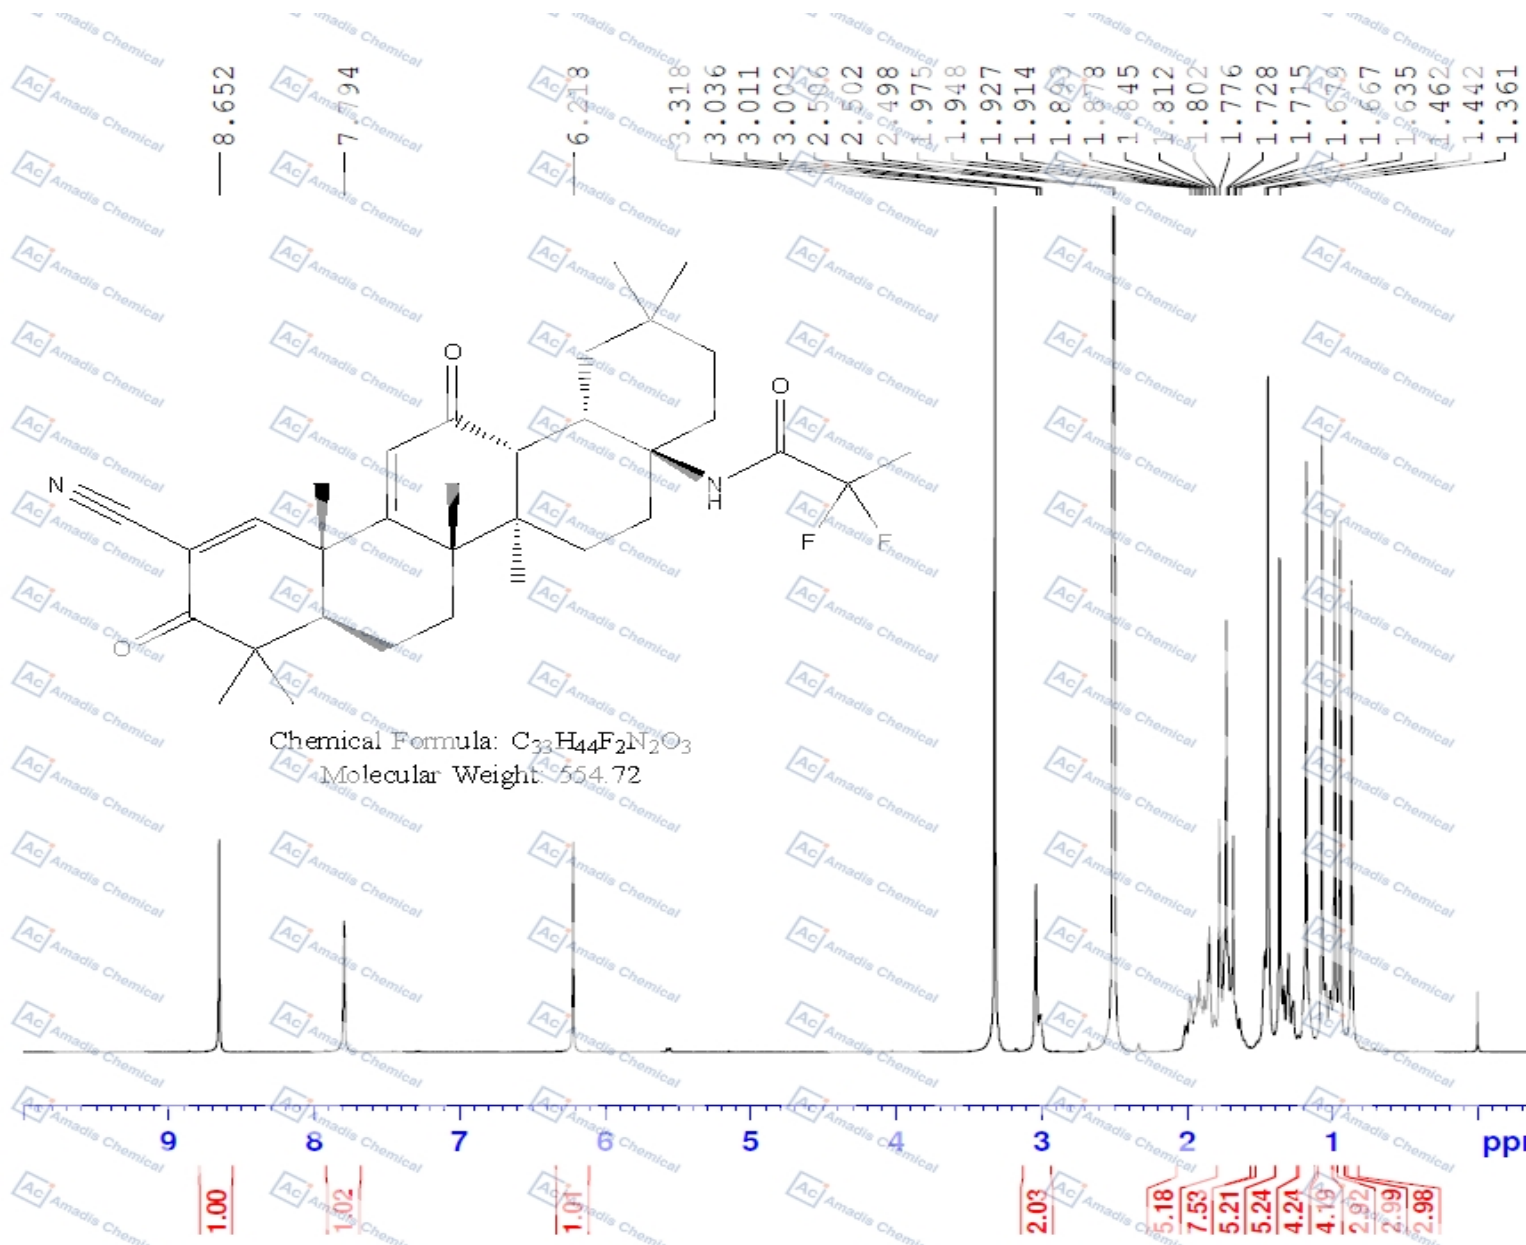

Current Data Parameters

NAME 1101-2032
EXPNO 1
PROCNO 1

F2 Acquisition Parameters

Date_ 20241104
Time 13:57
INSTRUM spect
PROBHD Z116098_0490 (12530
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 4
SWH 8012.820 MHz
FIDRES 0.244532 Hz
AQ 4.089465 sec
RG 786.19
DW 62.400 usec
DE 6.50 usec
TE 293.4 K
D1 1.0000000 sec
TDC 1
SFO1 400.1524709 MHz
NUC1 1H
PC1 10.00 usec
PL1 14.6979999 W

F2 - Processing parameters

SF 655.36 MHz
SE 400.1500026 MHz
WDW EM
SSB 0
LA 30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.