


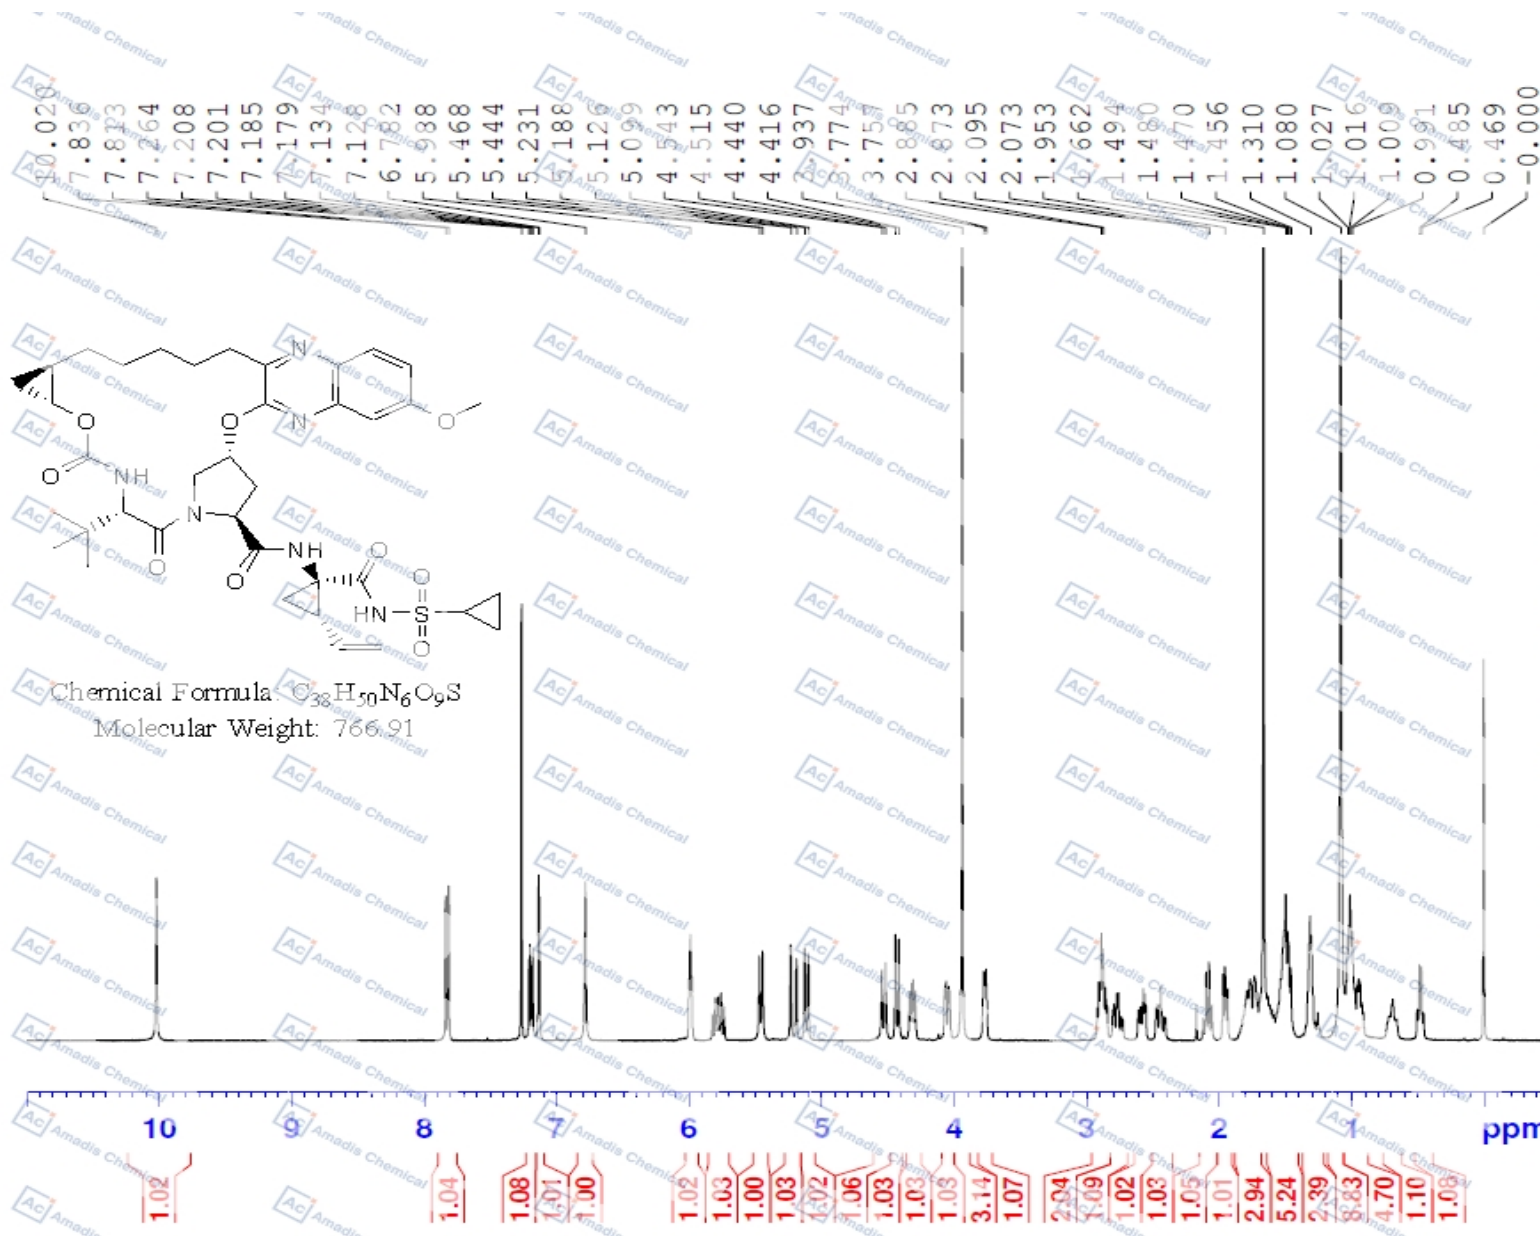

Current Data Parameters
NAME 1010-4999
EXPNO 10
PROCNO 10

F2 - Acquisition Parameters
Date_ 20241011
Time 11:23 h
INSTRUM spect
PROBHD 116098_0490 (zq30)
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 8012.920 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 111.92
DW 62.400 usec
DE 6.50 usec
TE 298.3 K
D1 1.00000000 sec
TD 65536
SFO 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 14.6979992 W

F2 - Processing parameters
SI 65536
SF 400.1500009 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.