


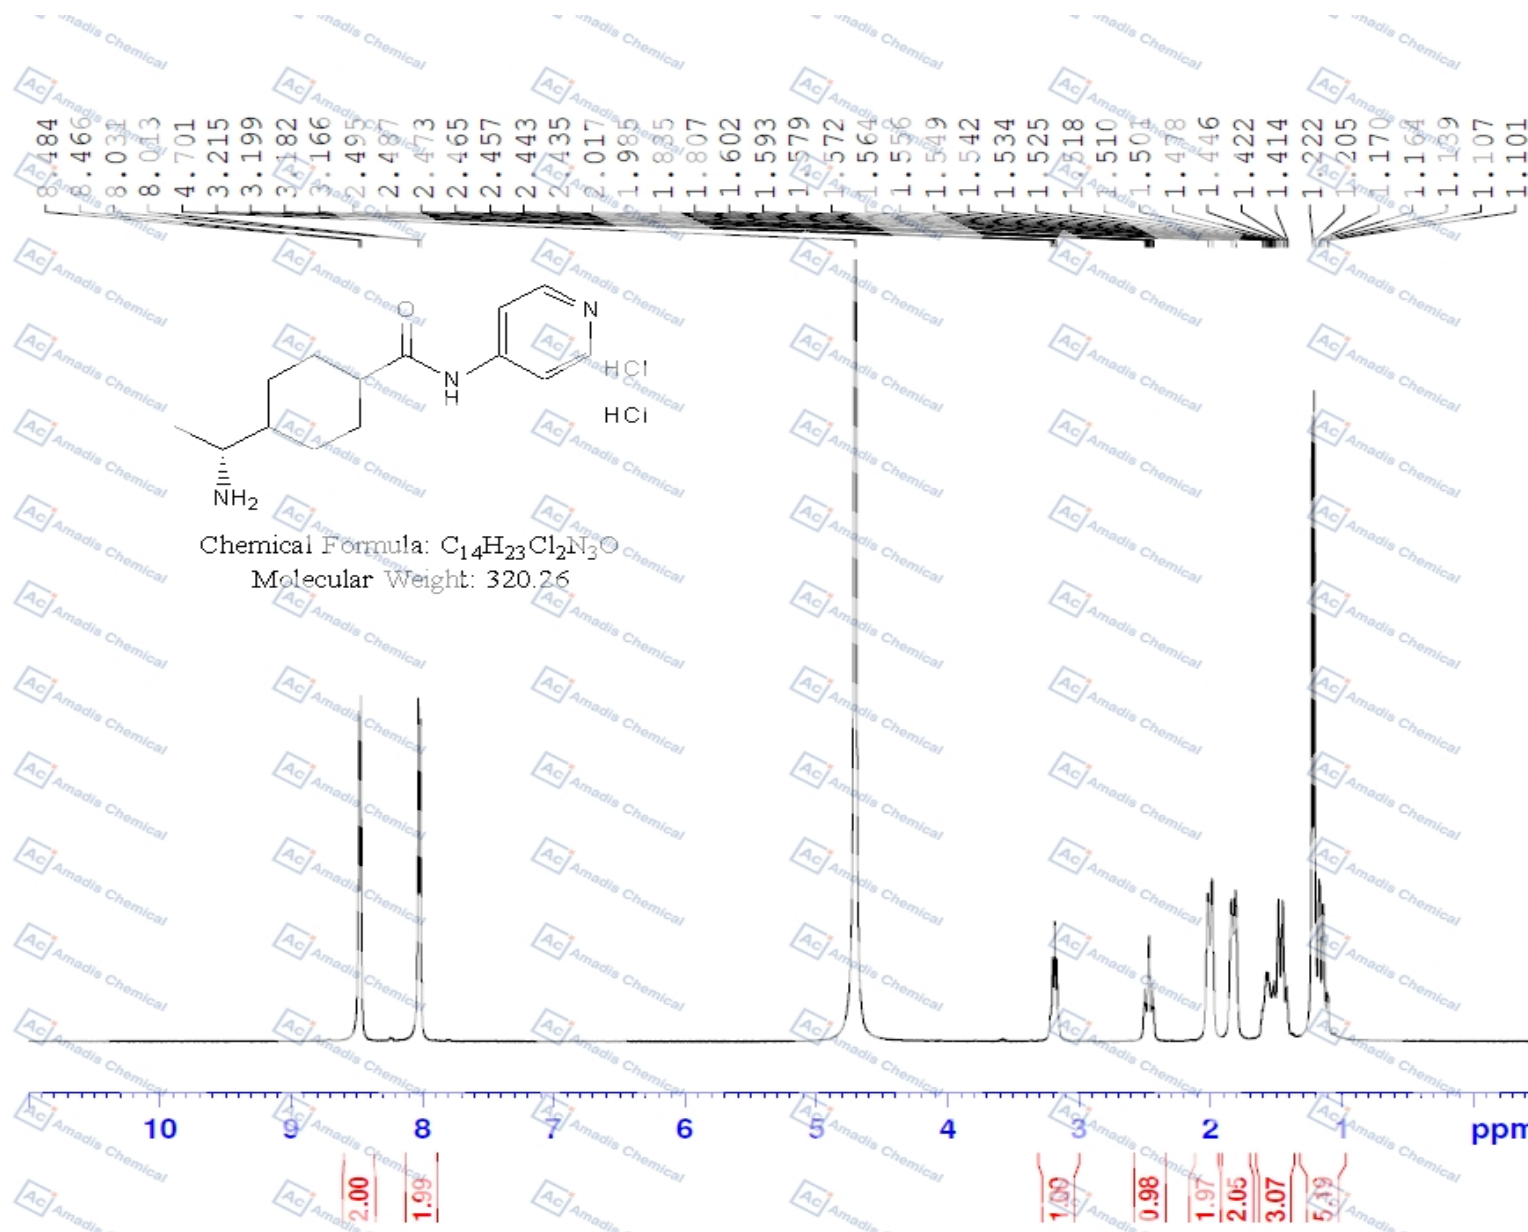

Current Data Parameters
NAME 1023-5020
EXPNO 0
PROCNO 0

F2 - Acquisition Parameters

Date_ 20241004
Time 12.29 h
INSTRUM spect
PROBHD 16098_0490 (1H/13C)
PULPROG zgpg30
TD 65536
SOLVENT D2O
NS 16
DS 2
SWH 8012.826 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 123.07
DW 62.408 usec
DE 6.50 usec
TE 298.9 K
D1 1.0000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PIPA 14.6979999 W

F2 - Processing parameters

SI 65536
SF 400.1500009 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.