


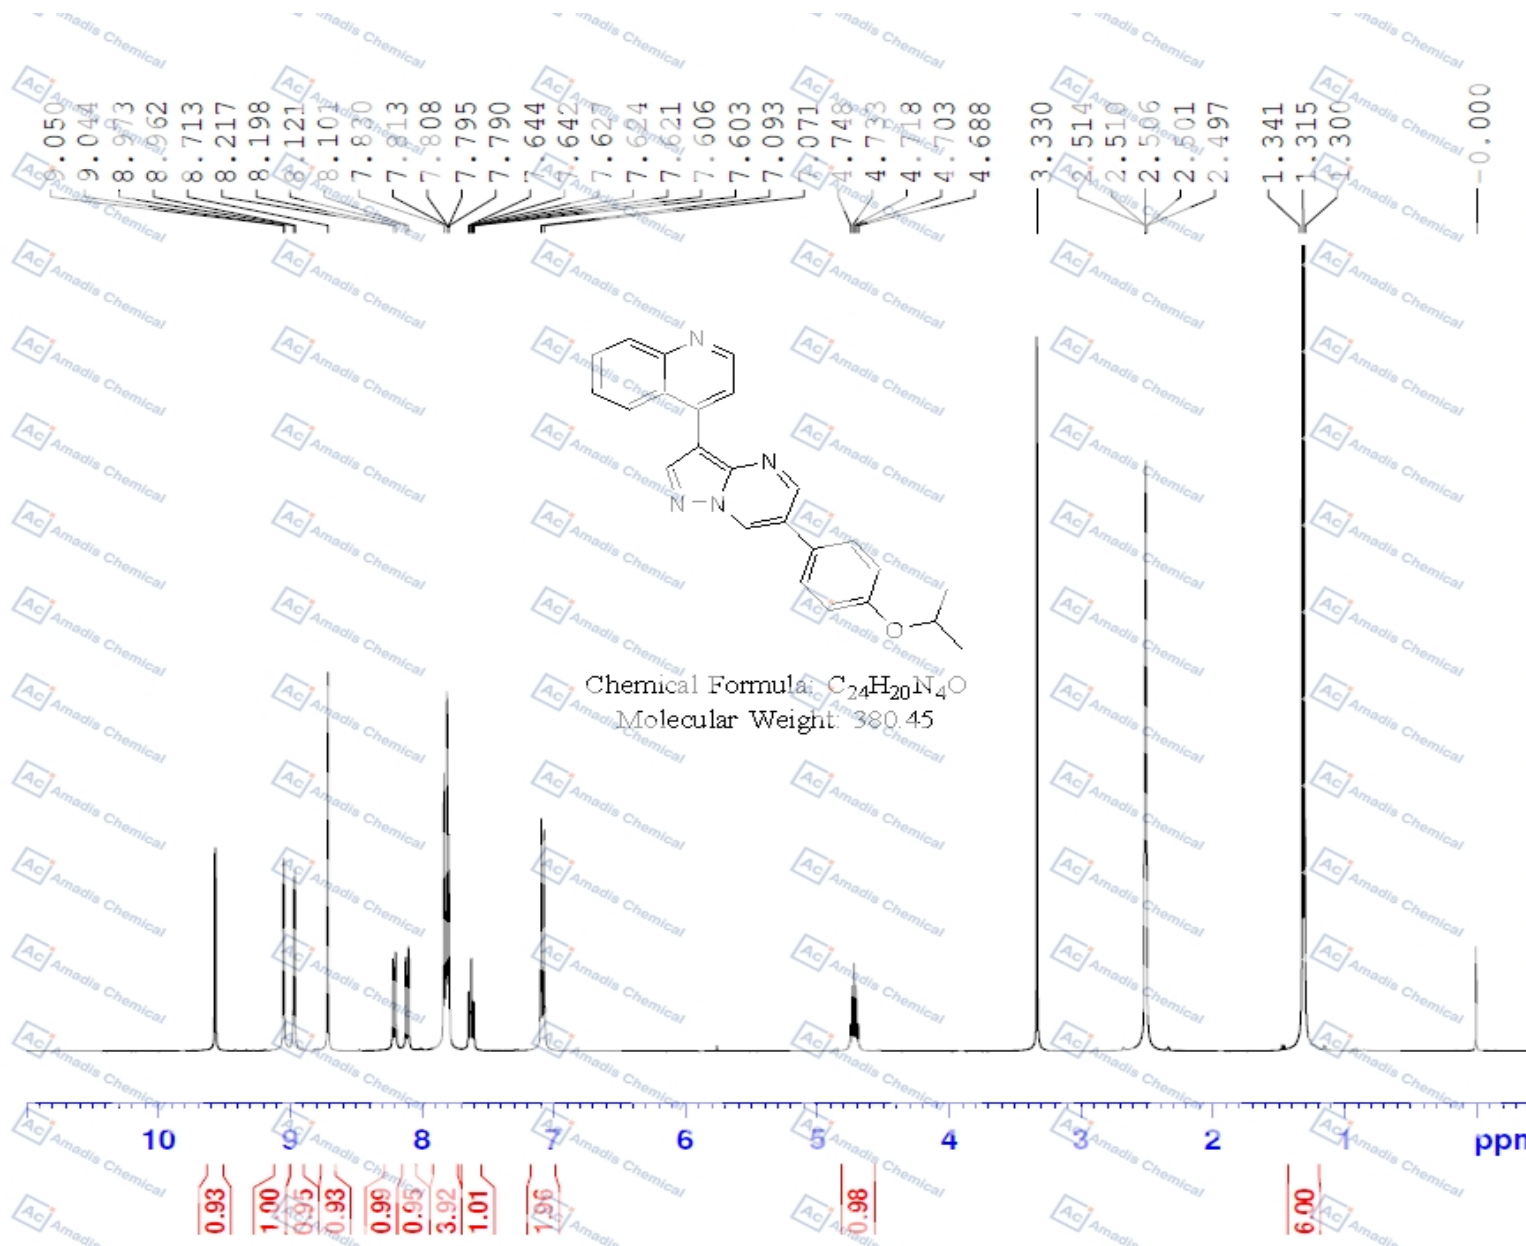

Current Data Parameters
NAME 0526-5309
EXPNO 10
PROCNO

F2 - Acquisition Parameters
Date_ 20250527
Time 11:49 h
INSTRUM spect
PROBHD CP16098_0490 (16098)
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.826 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 111.22
DW 62.106 usec
DE 6.50 usec
TE 298.5 K
D1 1.0000000 sec
TDC 0.0000000 sec
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PIW 15.5930004 W

F2 - Processing parameters
SI 65536
SF 400.1500009 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.