



Current Data Parameters


EXPNO	1
PROCNO	1

F2 - Acquisition Parameters

Date_	20240430
Time	14.35 h
INSTRUM	Avance NEO
PROBHD	Z116098-0766 (
PULPROG	zg30
TD	65536
SF	400.1324708 MHz
WDW	EM
SSB	0
LB	0.30 Hz
GB	0
PC	1.00

F2 - Processing parameters

SI	65536
SF	400.1300139 MHz
WDW	EM
SSB	0
LB	0.30 Hz
GB	0
PC	1.00

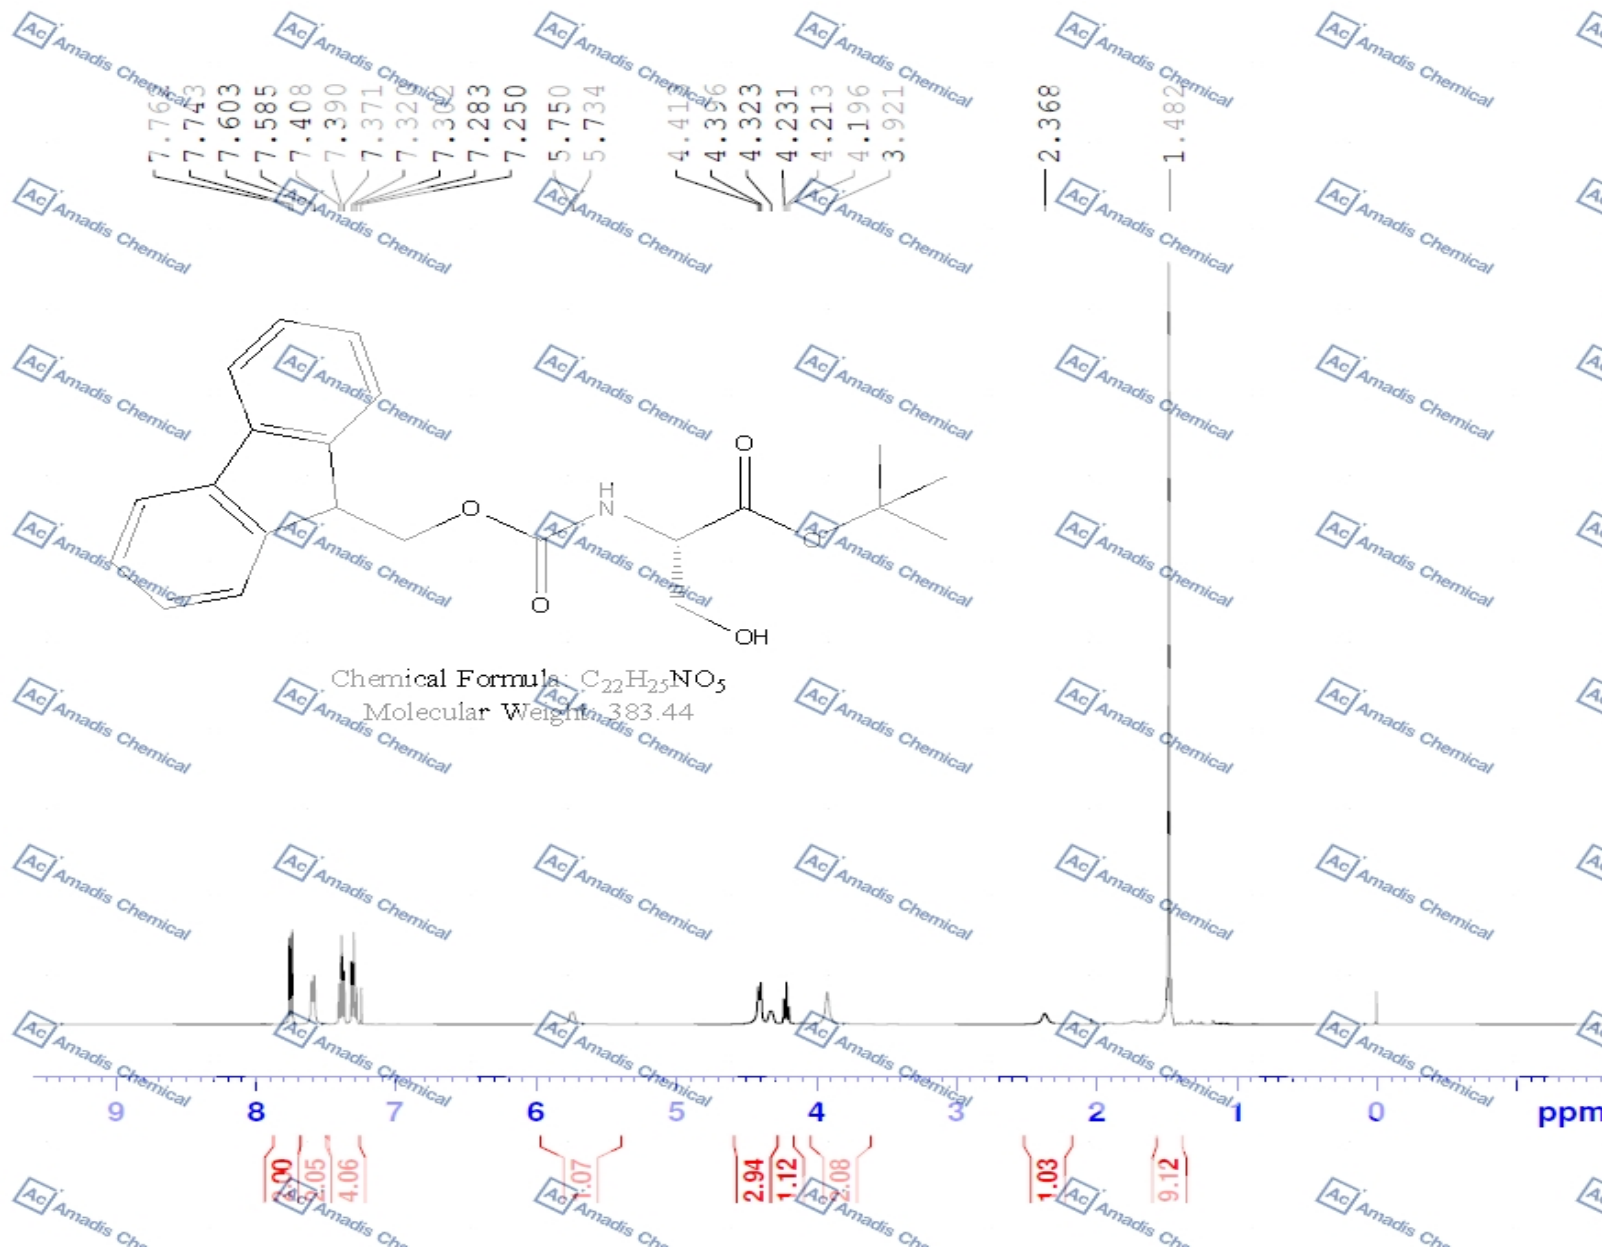

*For laboratory or manufacturing use only, not for drug, food and household use.