




Current Data Parameters
NAME 0613-48
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240614
Time 12.15 h
INSTRUM spect
PROBHD zgpg30
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 137
DW 62.400 usec
DE 6.50 usec
TE 298.4 K
D1 1.00000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PLW 14.6979995 MHz

F2 - Processing parameters
SI 65536
SF 400.1500090 MHz
WDW EM
SSB 0
LB 0.20 Hz
GB 0
PC 1.00

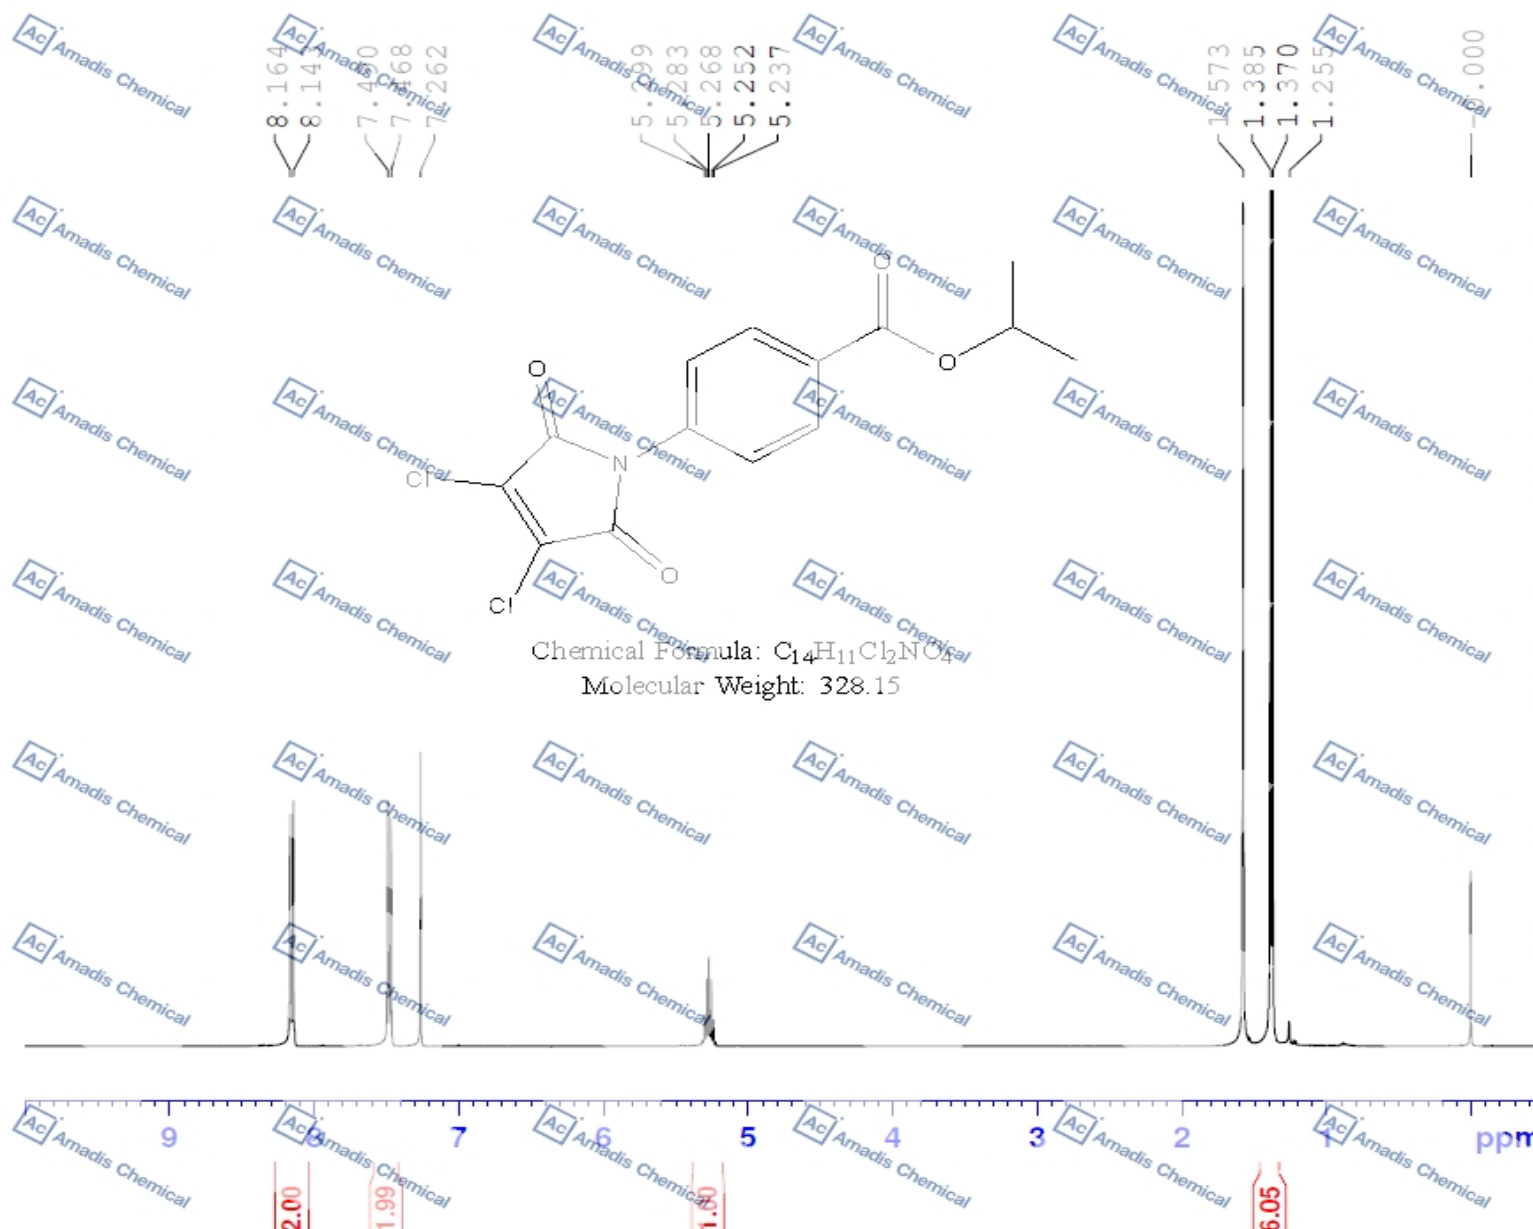

*For laboratory or manufacturing use only, not for drug, food and household use.