


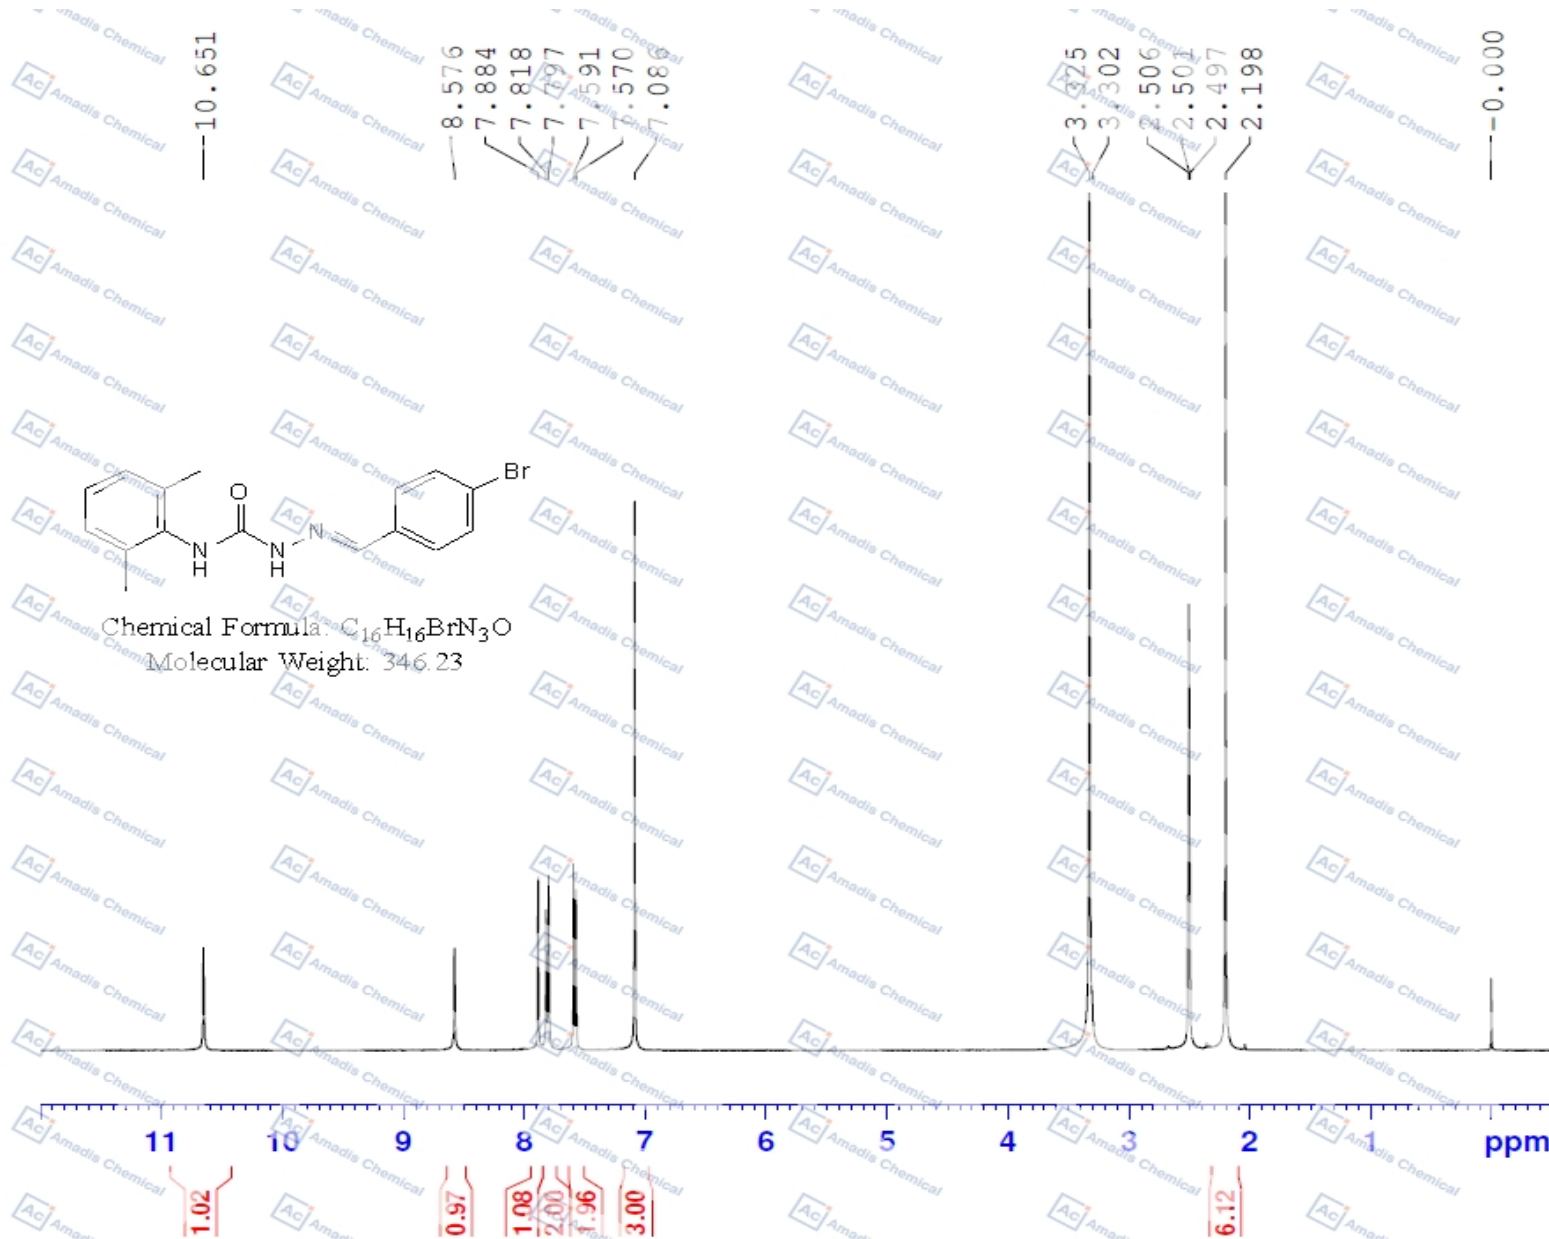

BRUKER

Current Data Parameters

NAME	0823-4942
EXPNO	1
PROCNO	1

F2 - Acquisition Parameters

Date_	20240826
Time	13:27 h
INSTRUM	spect
PROBHD	116098_0490 (
PULPROG	zg30
TD	65536
SOLVENT	DMSO
NS	16
DS	2
SWH	8012.400 Hz
FIDRES	0.244532 Hz
AQ	4.0894465 sec
RG	123.07
DE	62.400 usec
TE	298.5 K
D1	1.00000000 sec
TOU	
SFO1	400.1524703 MHz
NUC1	1H
P1	10.00 usec
PL1	14.6979995 W

F2 - Processing parameters

SI	65536
SPAC	400.1500834 MHz
WDW	EM
SSB	0
LB	0.30 Hz
GB	0
PC	1.00

*For laboratory or manufacturing use only, not for drug, food and household use.