




Current Data Parameters
NAME 0314-5177
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters

Date_ 20250317
Time 15:49:10
INSTRUM spect
PROBHD Z16098_0490 (4.00mm 1H/13C QNP) (1.5mm) (1.5mm)
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 127.87
DW 62.400 usec
DE 6.50 usec
TE 296.2 K
D1 1.00000000 sec
TDO
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PL1 0.00 dB
F1 15.59300041 W

F2 - Processing parameters

SI 65536
SF 400.1500026 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

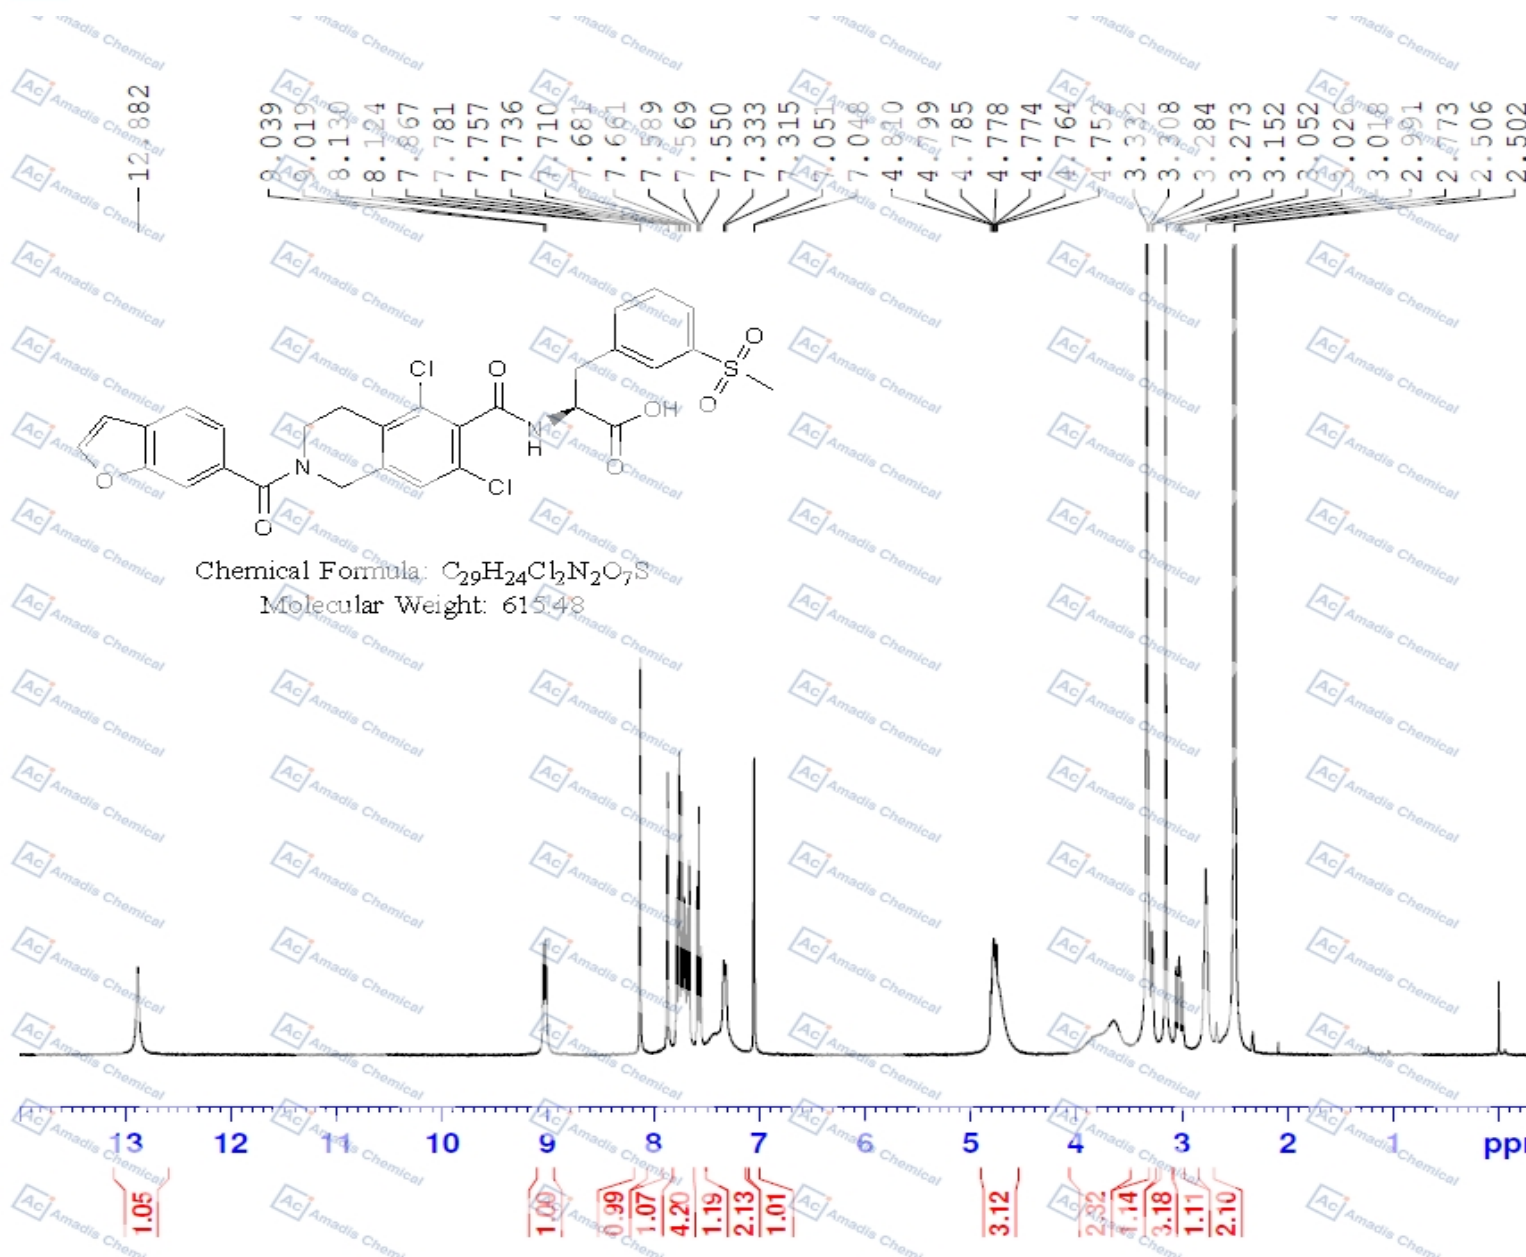

*For laboratory or manufacturing use only, not for drug, food and household use.