




Current Data Parameters
NAME 0509-4
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240510
Time 11.48 h
INSTRUM spect
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.089445 sec
RG 137
DW 62.400
DE 6.50 usec
TE 299.7 K
D1 1.0000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10 usec
PL1 14.6979952 dB

F2 - Processing parameters
SI 65536
SF 400.1500091 MHz
WDW EM
SSB 0
LB 0.20 Hz
GB 0
PC 1.00

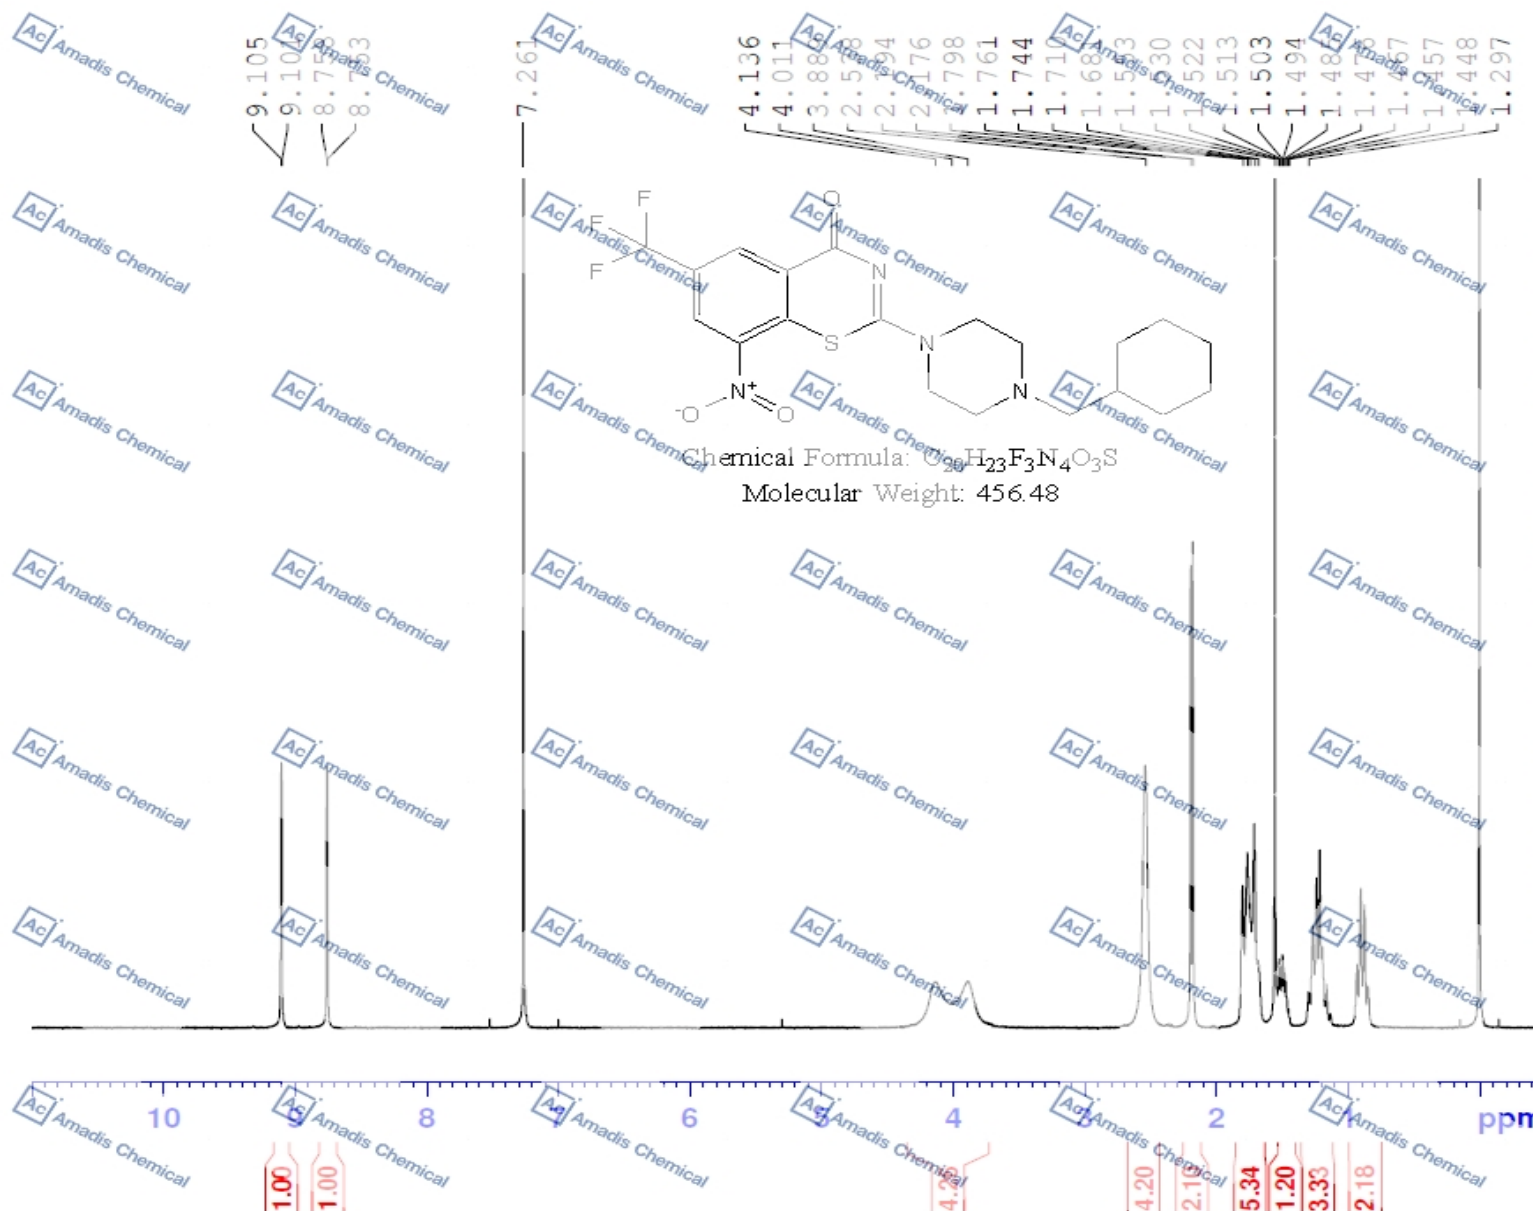

*For laboratory or manufacturing use only, not for drug, food and household use.