


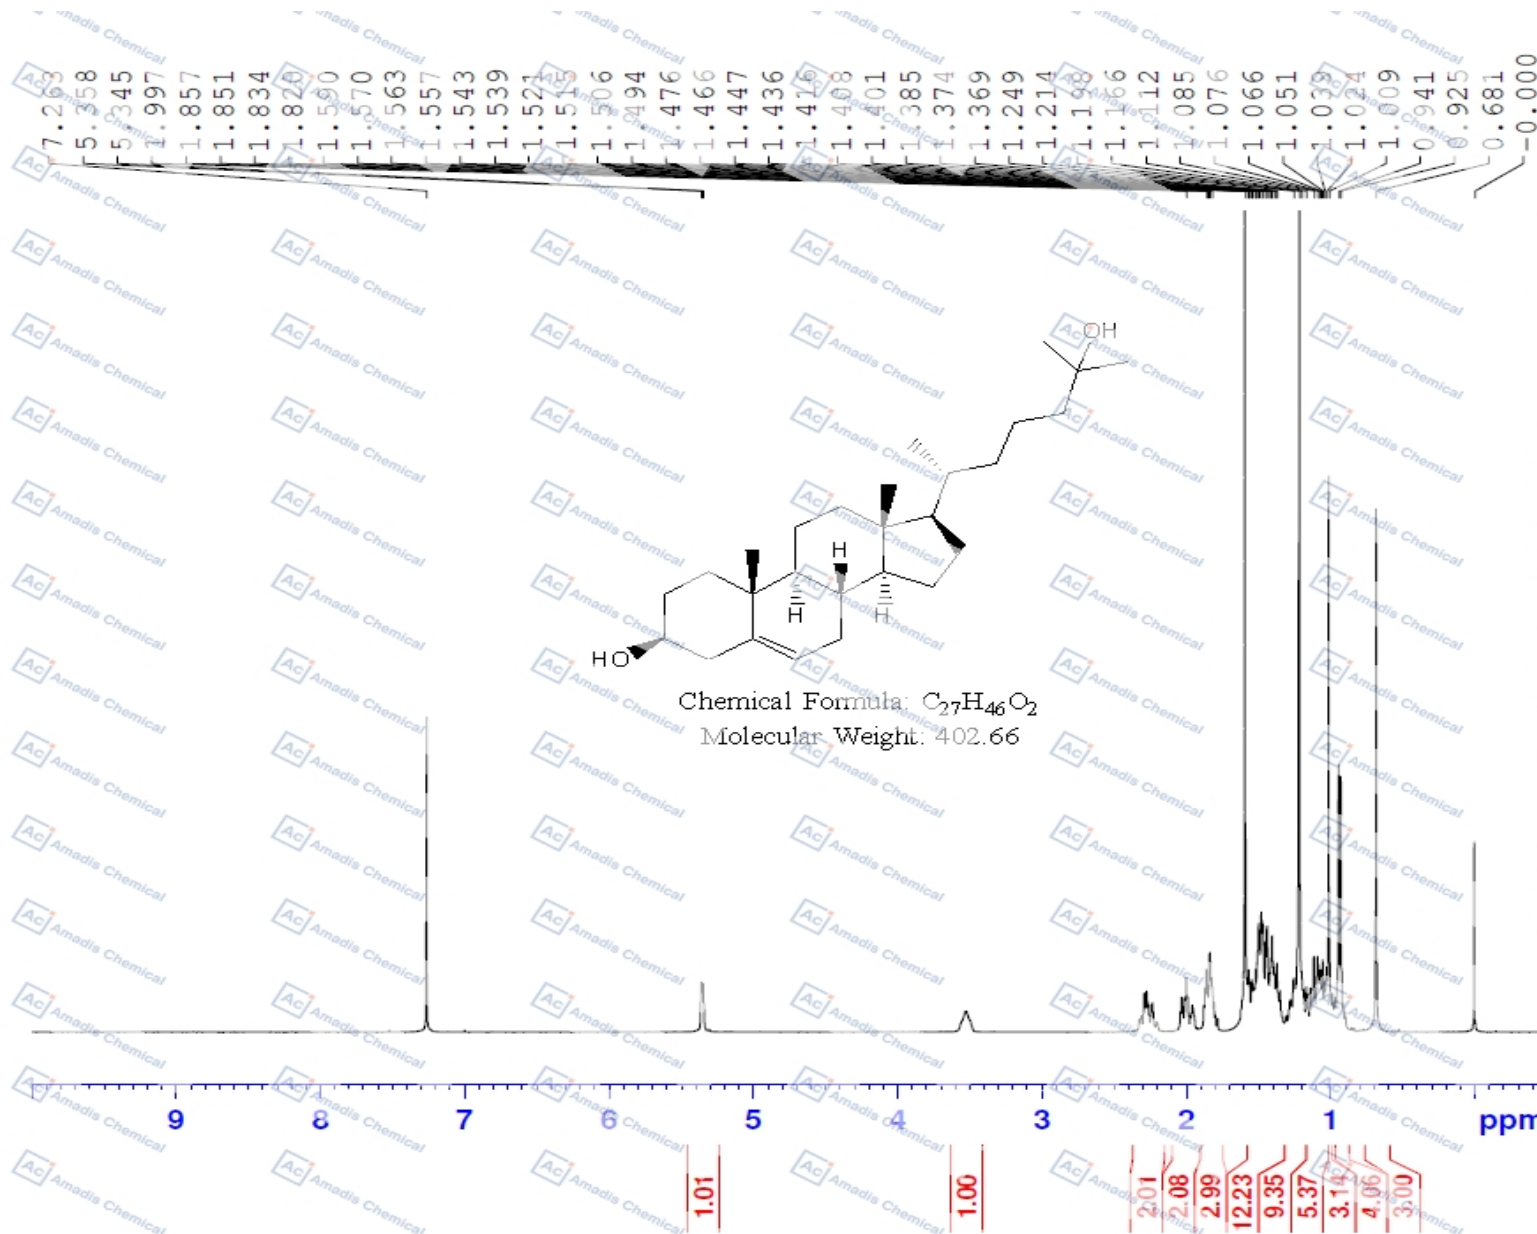

Current Data Parameters
NAME: 0805-4907
EXPNO: 10
PROCNO: 1

F2 Acquisition Parameters
Date_ 20240806
Time 11.36
INSTRUM spect
PROBHD zll6098_0490
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 4
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 111.92
DW 62.400 usec
DE 6.50 usec
TE 299.0 K
D1 1.0000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PLW1 14.6979995 W

F2 - Processing parameters
SI 65536
SF 400.1500036 MHz
WDW EM
SSP 0
LB 0.40 Hz
GB 0
PC 1.00

*For laboratory or manufacturing use only, not for drug, food and household use.