




Current Data Parameters
NAME 0527-4734
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240528
Time 10.47 h
INSTRUM spect
PROBHD z116098_0490
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 87
DW 62.50 usec
DE 6.50 usec
TE 299.3 K
D1 1.0000000 sec
TD0 1
SFO1 400.1524709 MHz
NUC1 1H
P1 10.00 usec
PR 14.6979999 W

F2 - Processing parameters
SI 65536
SF 400.1499901 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 1.00
PC 1.00

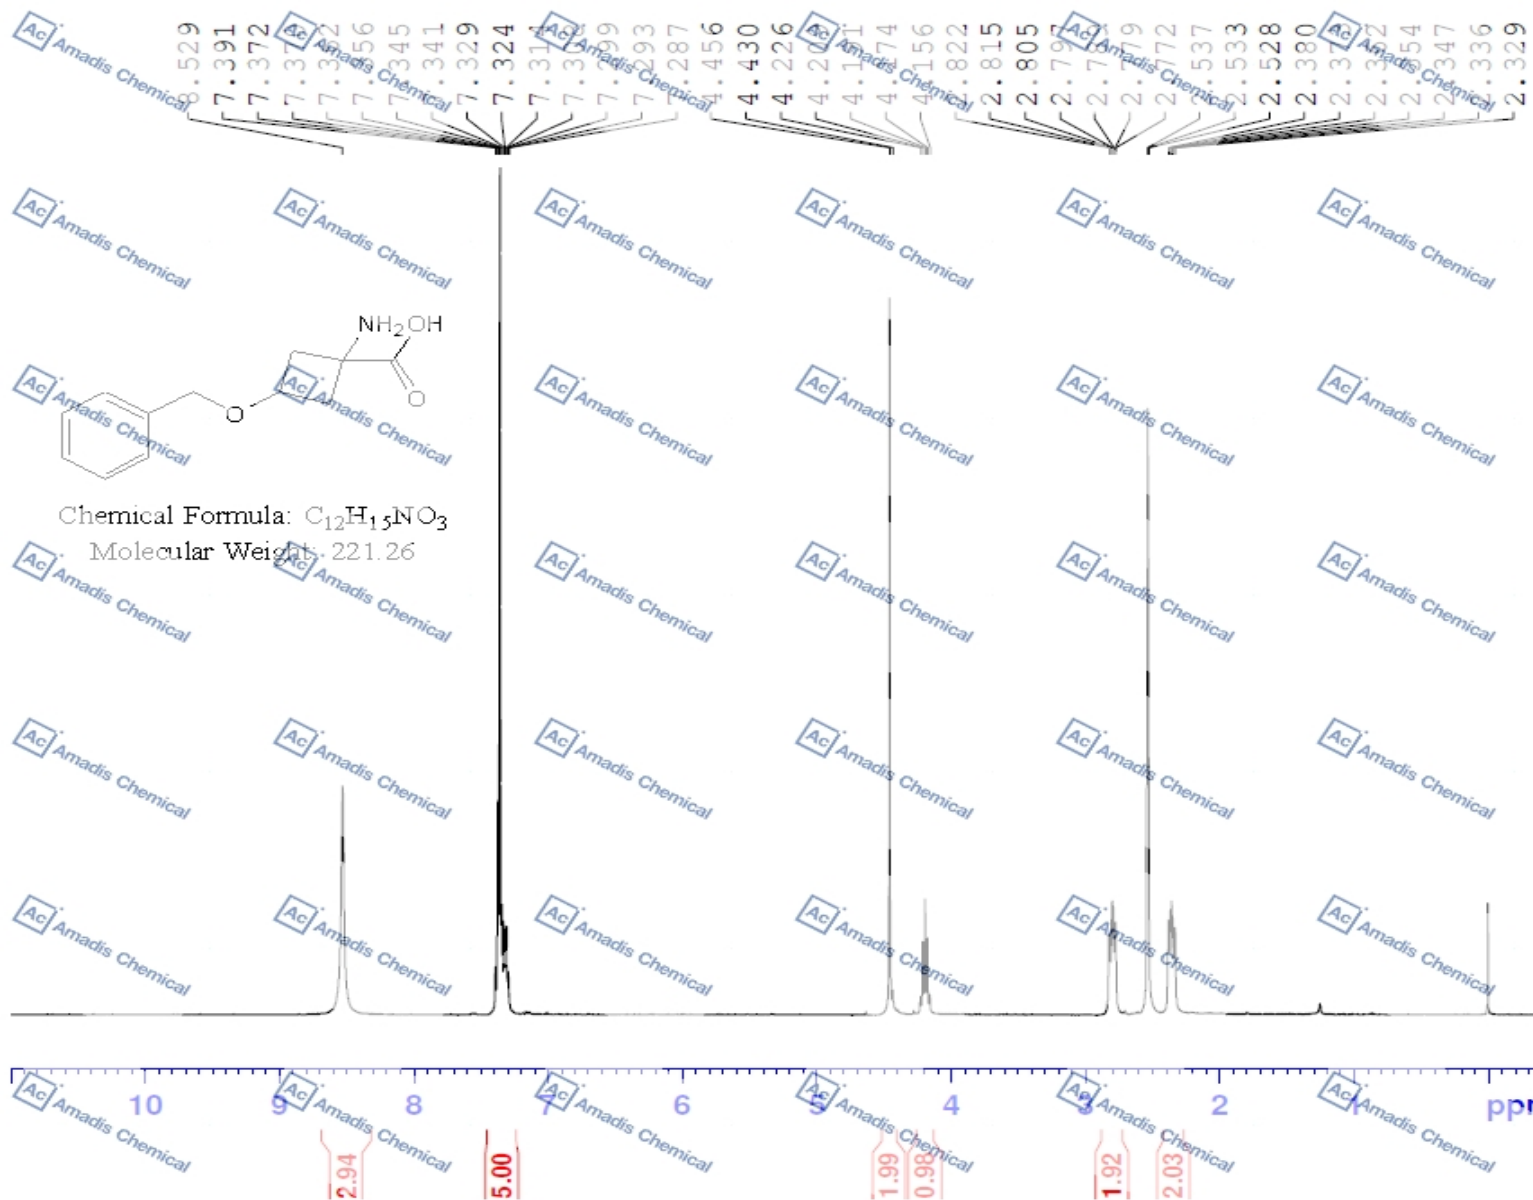

*For laboratory or manufacturing use only, not for drug, food and household use.