


HPLC of 23052-19-9

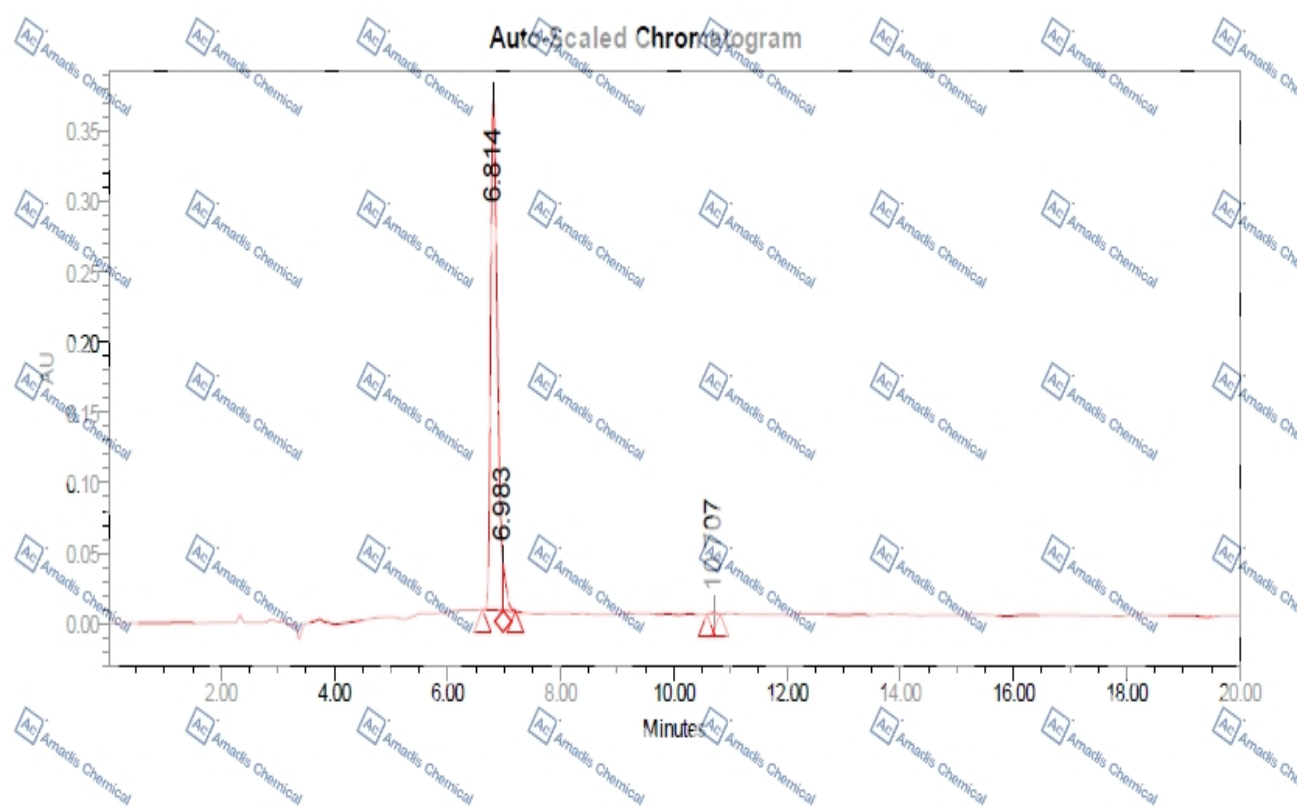

Peak Results

	RT	Area	Height	% Area	Channel Id
1	6.814	2963798	363813	95.54	40403
2	6.983	127070	33798	4.10	40403
3	10.707	11141	1635	0.36	40403

*For laboratory or manufacturing use only, not for drug, food and household use.

*if you have any comments and suggestions, please contact us by sales@amadischem.com