




Current Data Parameters
NAME 0526-5312
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250527
Time 11:52:40
INSTRUM spect
PROBHD Z146098_0490 (1H/13C)
PULPROG zgpg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.825 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 67.19
DW 62.400 usec
DE 6.50 usec
TE 298.4 K
D1 1.00000000 sec
TDS
SFO1 400.1524709 MHz
NUC1 1H
P1 10.60 usec
PL1 15.5930067 W

F2 - Processing parameters
SI 65536
SF 400.1500000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB
PC 1.00

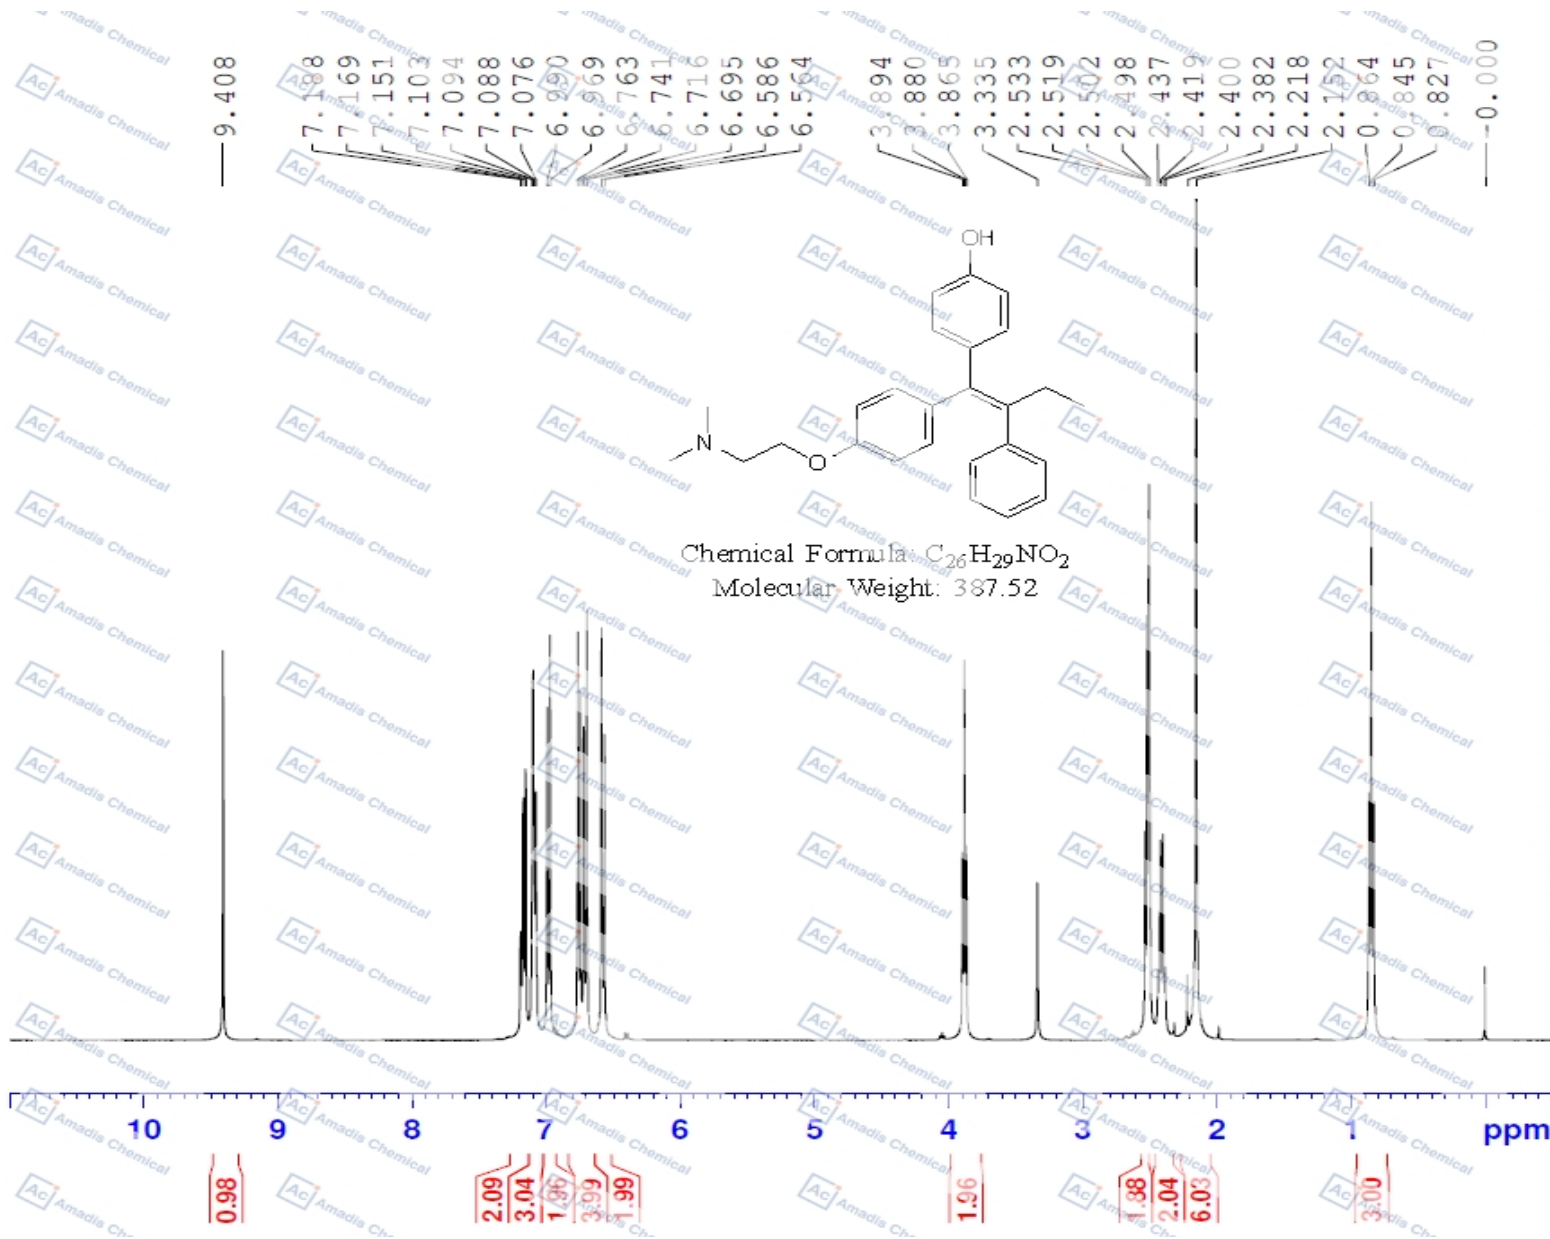

*For laboratory or manufacturing use only, not for drug, food and household use.